

IDENTIFYN RESOLUTION STEPDOWN

SECONDARY ANTIBODY MICROSCOPY EVIDENCE ASSESSMENT

Identifyn® SRM Alexa Fluor™ 680 Affinity Purified Donkey Anti-Mouse, IgG (H + L)

WESTERN BLOT -> WIDEFIELD -> WIDEFIELD SIM / APOTOME -> CONFOCAL -> AIRYSCAN
SIM -> SIM² -> SINGLE-MOLECULE STORM

8


ORDERED EVIDENCE TIERS

1

SUPPORTING CONTROL

PENDING

SCIENTIST REVIEW

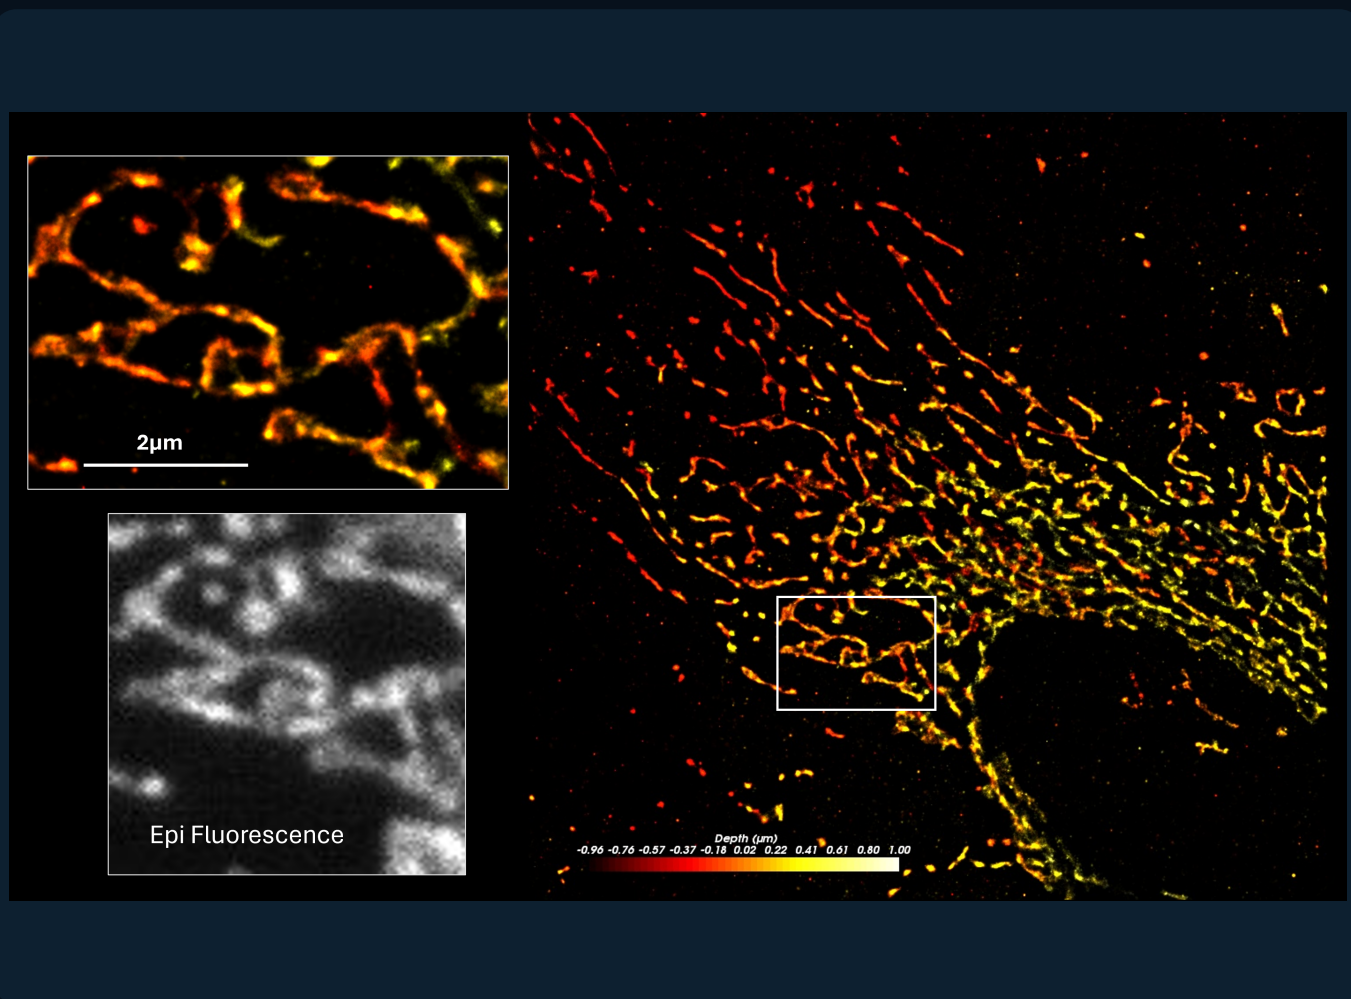

REPRESENTATIVE HIGHEST-AVAILABLE VIEW / SINGLE-MOLECULE STORM

SA-000070 | PRODUCT-LEVEL EVIDENCE DOSSIER

SOURCE-GROUNDED MICROSCOPY + BIOLOGICAL REVIEW / IDENTIFYN EVIDENCE PRESERVED

CRO CAPABILITY DEMONSTRATED

Identifyn performed the experimental and imaging work documented below. BENNETT converts that operating history into a governed, source-bounded scientific record.

- Source-documented sample preparation and antibody/reagent workflow
- Western blot imaging
- Widefield fluorescence microscopy
- Widefield structured illumination / Apotome optical sectioning
- Confocal microscopy
- Airyscan acquisition and reconstruction workflow
- Structured illumination microscopy
- SIM² reconstruction workflow
- Single-molecule STORM presentation workflow
- Preserved control experiment
- Z-stack / 3D acquisition
- Multi-channel imaging

SCIENTIFIC QUESTION

What source-bounded experimental and microscopy evidence is preserved for Identifyn® SRM Alexa Fluor™ 680 Affinity Purified Donkey Anti-Mouse, IgG (H + L), and what is the strongest interpretation allowed by the available modalities and controls?

EVIDENCE AVAILABLE

Western blot -> Widefield -> Widefield SIM — Apotome -> Confocal -> Airyscan -> SIM -> SIM² -> Single-molecule STORM
-> Control

BENNETT ASSESSMENT

The preserved SA-000070 record contains the full ordered evidence sequence from Western blot through single-molecule STORM. Each modality retains its own acquisition and processing boundary.

BENNETT / MICROSCOPY AND BIOLOGICAL EVIDENCE REVIEW

SOURCE-GROUNDED RETROSPECTIVE REVIEW / PENDING SCIENTIST REVIEW

SOURCE STATE	SOURCE HASH VERIFIED / EVENT RECORDED
BENNETT EVIDENCE REVIEW	COMPLETED / SOURCE-BOUNDED
NATIVE IMAGE REPROCESSING	NOT PERFORMED
LITERATURE SOURCES	INDEPENDENTLY VERIFIED
SCIENTIST REVIEW	PENDING
PUBLICATION	NOT AUTHORIZED

OVERALL CALL / FULL STEPDOWN / SOURCE-BOUNDED REVIEW

The preserved SA-000070 record contains the full ordered evidence sequence from Western blot through single-molecule STORM. Each modality retains its own acquisition and processing boundary.

SETTINGS ASSESSMENT

The record preserves 8 ordered evidence tier(s). Structured source metadata values are reported by stage and remain tied to the original method objects.

BIOLOGICAL SUPPORT

The record supports retrospective, source-bounded microscopy review. Target identity, specificity, treatment effect, binding, interaction and mechanism are not inferred from presentation images alone.

CONTROL ASSESSMENT

A true preserved control record is present and appears last.

CLAIM CEILING

This draft supports historical capability documentation, source registration, modality ordering, settings review and bounded interpretation. It does not independently validate antibody specificity, quantify a population response, establish binding, interaction, causation or mechanism, or authorize publication.

PROCESSING DISCLOSURE

Retrospective BENNETT architectural evaluation of preserved Identifyn source evidence. BENNETT did not perform native-file reprocessing, new deterministic measurement or the historical image post-processing represented in this record.

REAGENTS AND ACQUIRED CHANNELS

Preparation reagents are reported separately from channels actually documented in the acquisition settings. Fluorophores mentioned in staining are not automatically treated as acquired channels.

EVIDENCE OBJECT	REAGENTS / FLUOROPHORES PRESENT	CHANNELS ACTUALLY ACQUIRED
Western blot	680	Not deterministically stated in the acquisition block
Widefield	405/DAPI; 555; 680	3; 50 Cy5; 4AF532-49014; 49 DAPI; 625 - 655; 515 - 545; 335 - 383; 665 - 715
Widefield SIM — Apotome	405/DAPI; 532; 555; 680	3; 50 Cy5; AF532-49014; 49 DAPI; 625 - 655; 515 - 545; 335 - 383; 665 - 715
Confocal	405/DAPI; 488; 532; 680	3; None; 639nm @0.3%; 488nm @0.2%; 405nm @0.2%; 679; 493; 353
Airyscan	405/DAPI; 488; 680	2; None; 639nm @0.2%; 405nm @0.2%; 679; 353; 702; 465
SIM	405/DAPI; 488; 555; 680	3; SR HE LBF 405/488/561/642; 200 - 405, 200 - 488, 200 - 561, 200 - 642; 419 - 470, 503 - 546, 576 - 617, 657 - 800; T1-Axiocam 820 -SR; T2-Axiocam 820 #2-SR; T3-Axiocam 820 #2 -SR; 640
SIM ²	405/DAPI; 488; 555; 647; 680	3; SR HE LBF 405/488/561/642; 200 - 405, 200 - 488, 200 - 561, 200 - 642; 419 - 470, 503 - 546, 576 - 617, 657 - 800; T1-Axiocam 820 -SR; T2-Axiocam 820 #2-SR; T3-Axiocam 820 #2 -SR; 640
Single-molecule STORM	680	Both Channels
Control	405/DAPI; 680	2; 50 Cy5; 49 DAPI; 625 - 655; 335-383; 665 - 715; 420-470; 679

MODALITY ASSESSMENT / PART 1 OF 9

Western blot / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: Azure Sapphire FL. Objective: not explicitly stated. Platform: Azure Sapphire FL with Customizable Laser and Filter Modules, Enabling UV- NIR and Z-Plane(s). Structured source metadata values: 11.

VISIBLE OBSERVATION

A preserved presentation image is available for Western blot. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Western blot, documents platform context as Azure Sapphire FL, and records detected dye/channel descriptors as 680.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy and antibody-validation guidance that presentation evidence must remain bounded by modality, controls and source documentation.

INTERPRETIVE LIMIT

Band position and displayed intensity do not independently establish analytical specificity, target identity, linearity, or treatment effect.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Western blot evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 2 OF 9

Widefield / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS Axio Imager.M1. Objective: Plan-Apochromat 63x/1.40 Oil M27. Platform: Zeiss Axio Imager.M1 Widefield, using a Plan-Apochromat 63x/1.40 Oil M27, Axiocam 705, and X-Cite Xylis Lamp was used with the following parameters for each dye: Acquisition: Channels: 3; Scaling (Per Pixel): 0.102µm X 0.102µm; Image size (Pixels): 1388 X 1040; Image Size (Pixels): 1388 X 1040; Bit Depth: 12 Bit. Detector/camera: Imaging Device: Axiocam 705. Timing: Exposure Time: 400ms; 100ms. Illumination: Light source: X-Cite Xylis Lamp Intensity @30%; X-Cite Xylis Lamp Intensity @15%. Optical/scan: Effective NA: 1.4. Structured source metadata values: 38.

VISIBLE OBSERVATION

A preserved presentation image is available for Widefield. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Widefield, documents platform context as ZEISS Axio Imager.M1, and records detected dye/channel descriptors as 405/DAPI; 555; 680.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy and antibody-validation guidance that presentation evidence must remain bounded by modality, controls and source documentation.

INTERPRETIVE LIMIT

A presentation image supports gross localization and source-bounded co-occurrence, not direct binding, molecular colocalization, or native quantitative measurement.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Widefield evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 3 OF 9

Widefield SIM — Apotome / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS Axio Observer.Z1/7 Apotome. Objective: EC Plan-Neofluar 63X/1.25 oil M27. Platform: Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:. Acquisition: Z-Stack: 29 Slices (5.6µm); Channels: 3; Scaling (Per Pixel): 0.143µm X 0.143µm X 0.200µm; Image size (Pixels): 1037 X 1005; Image Size (Pixels): 1037 X 1005; Bit Depth: 14 Bit. Detector/camera: Imaging Device: Axiocam 807. Timing: Exposure Time: 380ms; 150ms. Illumination: Light source: X-Cite Xylis Lamp Intensity @85%; X-Cite Xylis Lamp Intensity @25%. Optical/scan: Effective NA: 1.25. Processing: Projection: View Angle 35°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected); Background: Black. Structured source metadata values: 47.

VISIBLE OBSERVATION

A preserved presentation image is available for Widefield SIM — Apotome. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Widefield SIM — Apotome, documents platform context as ZEISS Axio Observer.Z1/7 Apotome, and records detected dye/channel descriptors as 405/DAPI; 532; 555; 680.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy and antibody-validation guidance that presentation evidence must remain bounded by modality, controls and source documentation.

INTERPRETIVE LIMIT

Improved optical sectioning does not by itself establish reconstructed super-resolution or molecular interaction.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Widefield SIM — Apotome evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 4 OF 9

Confocal / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS LSM 980. Objective: Plan-Apochromat 63X/1.40 oil DIC M27. Platform: Zeiss LSM 980 Confocal with NIR Detection, Axio Observer.Z1/7, using a Plan-Apochromat 63X/1.40 oil DIC M27, was used with the following parameters for each dye:. Acquisition: Z-Stack: 62Slices (4.27µm); Channels: 3; Scaling (Per Pixel): 0.059µm X 0.059µm X 0.070µm; Image size (Pixels): 1612 X 1612; Image Size (Pixels): 1612 X 1612; Bit Depth: 16 Bit. Detector/camera: Imaging Device: GaAsP-Pmt 3; GaAsP-PMT 3; Detector Type: GaAsP-PMT. Timing: Pixel Time: 0.24µs; Frame Time: 6.04s. Illumination: Laser Wavelength: 639nm @0.3%; 488nm @0.2%. Optical/scan: Pinhole: 1.00AU / 67µm; 1.00AU / 49µm; Scan Zoom: 1.4; 1.1; LSM Scan Speed: 11; Scan Direction: Bidirectional; Averaging: 8; Effective NA: 1.4. Processing: Projection: View Angle 35°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected); Background: Black; LSM Plus Mode: 7.7 (3D, Auto); 7.3 (3D, Auto). Structured source metadata values: 57.

VISIBLE OBSERVATION

A preserved presentation image is available for Confocal. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Confocal, documents platform context as ZEISS LSM 980, and records detected dye/channel descriptors as 405/DAPI; 488; 532; 680.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy and antibody-validation guidance that presentation evidence must remain bounded by modality, controls and source documentation.

INTERPRETIVE LIMIT

Optical sectioning and source-bounded 3D presentation do not establish binding, mechanism, or population-level effect.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Confocal evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 5 OF 9

Airyscan / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS LSM 980. Objective: Plan-Apochromat 63X/1.40 oil DIC M27. Platform: Zeiss LSM 980 Confocal with NIR Detection, Axio Observer.Z1/7, using a Plan-Apochromat 63X/1.40 oil DIC M27, was used with the following parameters for each dye:. Acquisition: Z-Stack: 73 Slices (3.60µm); Channels: 2; Scaling (Per Pixel): 35.30nm X 35.30nm X 50.00nm; Image size (Pixels): 1793 X 1793; Image Size (Pixels): 1793 X 1793; Bit Depth: 16 Bit. Detector/camera: Imaging Device: Airyscan; Detector Type: GaAsP-PMT. Timing: Pixel Time: 1.15µs; Frame Time: 8.93s. Illumination: Laser Wavelength: 639nm @0.2%; 405nm @0.2%. Optical/scan: Pinhole: 5.00AU / 328µm; 5.46AU / 235µm; Scan Zoom: 2.1; LSM Scan Speed: 6; Scan Direction: Bidirectional; Effective NA: 1.4. Processing: Projection: View Angle 35°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected); Background: Black; AiryScan Mode: Super Resolution 9.5 (3D, Auto); Super Resolution 7.8 (3D, Auto). Structured source metadata values: 47.

VISIBLE OBSERVATION

A preserved presentation image is available for Airyscan. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Airyscan, documents platform context as ZEISS LSM 980, and records detected dye/channel descriptors as 405/DAPI; 488; 680.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy guidance that advanced-resolution outputs remain dependent on acquisition, reconstruction or localization quality control.

INTERPRETIVE LIMIT

Displayed feature separation remains reconstruction dependent; no unsupported numerical resolution or molecular architecture claim is permitted.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Airyscan evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 6 OF 9

SIM / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS Elyra. Objective: Plan-Apochromat 63X/1.40 oil DIC M27. Platform: Zeiss Elyra 5 Lattice SIM, AxioObserver.Z1/ 7 using Plan-Apochromat 63X/1.40 oil DIC M27, 1X Tubelens, was used with the following parameters for each dye:. Acquisition: Z-Stack: 68 Slices (3.35µm); Channels: 3; Scaling (Per Pixel): 13.20nm X 13.20nm X 50.00nm; Image size (Pixels): 2180 X 2828; Image Size (Pixels): 2180 X 2828; Bit Depth: 16 Bit. Detector/camera: Imaging Device: AxioCam 820; AxioCam 820 #2. Timing: Exposure Time: 150ms; 100ms; Frame Time: 1.98s; 1.33s. Illumination: Laser Wavelength: 640nm @8.0%; 561nm @1.00%; Illumination Wavelength: 640; 561. Optical/scan: Scan Direction: Unidirectional; Effective NA: 1.4. Processing: Algorithm: SIM; Process Sampling: N/A; Result Sampling: 4; Projection: View Angle 35°, Scale Z 86%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected); Background: Black. Structured source metadata values: 59.

VISIBLE OBSERVATION

A preserved presentation image is available for SIM. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as SIM, documents platform context as ZEISS Elyra, and records detected dye/channel descriptors as 405/DAPI; 488; 555; 680.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy guidance that advanced-resolution outputs remain dependent on acquisition, reconstruction or localization quality control.

INTERPRETIVE LIMIT

Reconstruction-dependent structural separation requires native reconstruction QC before numerical resolution or molecular dimensions can be claimed.

CLAIM CEILING

This tier supports a source-bounded statement that the historical SIM evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 7 OF 9

SIM² / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS Elyra. Objective: Plan-Apochromat 63X/1.40 oil DIC M27. Platform: Zeiss Elyra 5 Lattice SIM, AxioObserver.Z1/ 7 using Plan-Apochromat 63X/1.40 oil DIC M27, 1X Tubelens, was used with the following parameters for each dye:. Acquisition: Z-Stack: 54 Slices (2.65µm); Channels: 3; Scaling (Per Pixel): 13.20nm X 13.20nm X 50.00nm; Image size (Pixels): 5056 X 5056; Image Size (Pixels): 5056 X 5056; Bit Depth: 16 Bit. Detector/camera: Imaging Device: AxioCam 820; AxioCam 820 #2. Timing: Exposure Time: 150ms; 100ms; Frame Time: 1.98s; 1.33s. Illumination: Laser Wavelength: 640nm @8.0%; 561nm @1.00%; Illumination Wavelength: 640; 561. Optical/scan: Scan Direction: Unidirectional; Effective NA: 1.4. Processing: Algorithm: SIM2; Process Sampling: 4; Result Sampling: 4; Projection: View Angle 35°, Scale Z 275%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected); Background: Black. Structured source metadata values: 63.

VISIBLE OBSERVATION

A preserved presentation image is available for SIM². BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as SIM², documents platform context as ZEISS Elyra, and records detected dye/channel descriptors as 405/DAPI; 488; 555; 647; 680.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy guidance that advanced-resolution outputs remain dependent on acquisition, reconstruction or localization quality control.

INTERPRETIVE LIMIT

Further reconstruction-dependent segmentation does not establish molecular dimensions, structure identity, or mechanism without independent support.

CLAIM CEILING

This tier supports a source-bounded statement that the historical SIM² evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 8 OF 9

Single-molecule STORM / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: Bruker Vutara VXL. Objective: Olympus 60X/1.30 silicon oil objective. Platform: Bruker Vutara VXL Biplane Single Molecule Microscope, using an Olympus 60X/1.30 silicon oil objective, was used with the following parameters:.

Detector/camera: Camera: Both Cameras. Timing: Exposure Time: 20ms Selected; Super Resolution Camera Exposure Time: 20ms; Widefield Camera Exposure Time: 200ms. Illumination: Photoactivation/Imaging Laser: 0% Selected.

Structured source metadata values: 71.

VISIBLE OBSERVATION

A preserved presentation image is available for Single-molecule STORM. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Single-molecule STORM, documents platform context as Bruker Vutara VXL, and records detected dye/channel descriptors as 680.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy guidance that advanced-resolution outputs remain dependent on acquisition, reconstruction or localization quality control.

INTERPRETIVE LIMIT

Without localization tables, uncertainty, blinking, drift, and independent cluster evidence, the presentation cannot establish molecule count, cluster truth, exact precision, or molecular architecture.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Single-molecule STORM evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 9 OF 9

Control / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS Axio Observer.Z1/7 Apotome. Objective: EC Plan-Neofluar 63X/1.25 oil M27. Platform: Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, AxioCam 807, and X-Cite Xylys Lamp was used with the following parameters for each dye: Acquisition: Channels: 2; Scaling (Per Pixel): 0.143µm X 0.143µm; Image size (Pixels): 1067 X 686; Image Size (Pixels): 1067 X 686; Bit Depth: 14 Bit. Detector/camera: Imaging Device: AxioCam 807. Timing: Exposure Time: 300ms; 30ms. Illumination: Light source: X-Cite Xylys Lamp Intensity @25%; X-Cite Xylys Lamp Intensity @10%. Optical/scan: Effective NA: 1.25. Structured source metadata values: 32.

VISIBLE OBSERVATION

A preserved presentation image is available for Control. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Control, documents platform context as ZEISS Axio Observer.Z1/7 Apotome, and records detected dye/channel descriptors as 405/DAPI; 680.

LITERATURE CORRELATION

Consistent with peer-reviewed antibody-control guidance that a no-primary or related control bounds background but is not a complete specificity system.

INTERPRETIVE LIMIT

A control bounds the recorded comparison only; it does not establish universal specificity, zero background, zero cross-reactivity, or absence of free dye.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Control evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

CROSS-MODALITY SYNTHESIS

The preserved SA-000070 record contains the full ordered evidence sequence from Western blot through single-molecule STORM. Each modality retains its own acquisition and processing boundary.

Different acquisitions are not treated as a quantitative intensity ladder. Any continuity statement remains qualitative and source bounded.

BENNETT LITERATURE CORRELATION — SOURCES INDEPENDENTLY VERIFIED

BENNETT uses independently verified primary scientific sources to test whether the interpretation is scientifically consistent and properly bounded. Literature correlation does not retroactively validate the Identifyn dataset or replace scientist review.

- Antibody and microscopy evidence require orthogonal controls and modality-appropriate interpretation; presentation images alone do not establish analytical specificity.
- Advanced-resolution presentation depends on acquisition, reconstruction or localization quality control before numerical resolution, molecular dimensions or cluster identity can be claimed.

REFERENCES

1. Uhlen M, et al. A proposal for validation of antibodies. Nat Methods. 2016;13:823-827. doi:10.1038/nmeth.3995.
2. Gustafsson MGL. Surpassing the lateral resolution limit by a factor of two using structured illumination microscopy. J Microsc. 2000;198:82-87. doi:10.1046/j.1365-2818.2000.00710.x.
3. Sage D, et al. Quantitative evaluation of software packages for single-molecule localization microscopy. Nat Methods. 2015;12:717-724. doi:10.1038/nmeth.3442.

RELEASE BOUNDARY

This assessment remains a draft pending scientist review. No publication is authorized. Any future native-file analysis must enter BENNETT as a new evidence snapshot with routed engine authority, native-data QA, methods, limitations, and an independently reviewed claim ceiling.

SOURCE RECONCILIATION / QA / PROVENANCE

SOURCE STATUS - PRESERVED / AUTO-RECONCILED

Historical Identifyn source material was subjected to BENNETT retrospective QA. Original source state and correction history remain preserved in provenance.

HIGH CONFIDENCE - AUTO-RECONCILED

Airyscan / Scaling (Per Pixel): 35.30nm X 35.30nm X 50.00nm -> 0.03530 μm X 0.03530 μm X 0.05000 μm . Both numerical magnitude and unit were normalized, then checked against the reported field dimensions; no unit label was changed alone. Supporting evidence: Image Size (Pixels)=1793 X 1793; Image Size (Scaled)=63.29 μm X 63.29 μm ; PASS - INTERNALLY CONSISTENT. Documented sampling reproduces the reported physical field dimensions. Maximum field-dimension error 0.00%.

HIGH CONFIDENCE - AUTO-RECONCILED

SIM / Scaling (Per Pixel): 13.20nm X 13.20nm X 50.00nm -> 0.01320 μm X 0.01320 μm X 0.05000 μm . Both numerical magnitude and unit were normalized, then checked against the reported field dimensions; no unit label was changed alone. Supporting evidence: Image Size (Pixels)=2180 X 2828; Image Size (Scaled)=28.77 μm X 37.32 μm ; PASS - INTERNALLY CONSISTENT. Documented sampling reproduces the reported physical field dimensions. Maximum field-dimension error 0.03%.

HIGH CONFIDENCE - AUTO-RECONCILED

SIM² / Scaling (Per Pixel): 13.20nm X 13.20nm X 50.00nm -> 0.01320 μm X 0.01320 μm X 0.05000 μm . Both numerical magnitude and unit were normalized, then checked against the reported field dimensions; no unit label was changed alone. Supporting evidence: Image Size (Pixels)=5056 X 5056; Image Size (Scaled)=66.72 μm X 66.72 μm ; PASS - INTERNALLY CONSISTENT. Documented sampling reproduces the reported physical field dimensions. Maximum field-dimension error 0.03%.

BENNETT EVIDENCE REVIEW COMPLETE

INTERPRETATION TO EVIDENCE

BENNETT has completed the bounded retrospective assessment.
The following pages switch ownership to the preserved Identifyn record.



IDENTIFYN PRESERVED SOURCE EVIDENCE

ORIGINAL RECORD BEGINS

Images, source methods, acquisition settings and provenance follow in the locked Stepdown order. Scientific wording is preserved; missing modalities are not invented. A preserved control follows all available Stepdown tiers as supporting evidence.

PRODUCT-LEVEL STEPDOWN MAP


This dossier preserves the complete available evidence progression for SA-000070. Each tier remains tied to its original image, source method, instrument context and cryptographic identity. A preserved control is retained as supporting evidence and appears after every resolution tier.

CANONICAL STEPDOWN	EVIDENCE STAGE	INSTRUMENT	STATUS
1	Western blot	Azure Sapphire FL	PRESERVED
2	Widefield	ZEISS Axio Imager.M1	PRESERVED
3	Widefield SIM - Apotome	ZEISS Axio Observer.Z1/7 Apotome	PRESERVED
4	Confocal	ZEISS LSM 980	PRESERVED
5	Airyscan	ZEISS LSM 980	PRESERVED
6	SIM	ZEISS Elyra	PRESERVED
7	SIM ²	ZEISS Elyra	PRESERVED
8	Single-molecule STORM	Bruker Vutara VXL	PRESERVED

INTERPRETIVE BOUNDARY

Ordering evidence by resolution tier does not make the modalities interchangeable. Each stage retains its acquisition environment and scientific limitations. This pilot organizes the record; it does not synthesize new biological claims.

ORIGINAL IMAGE EVIDENCE / WESTERN BLOT

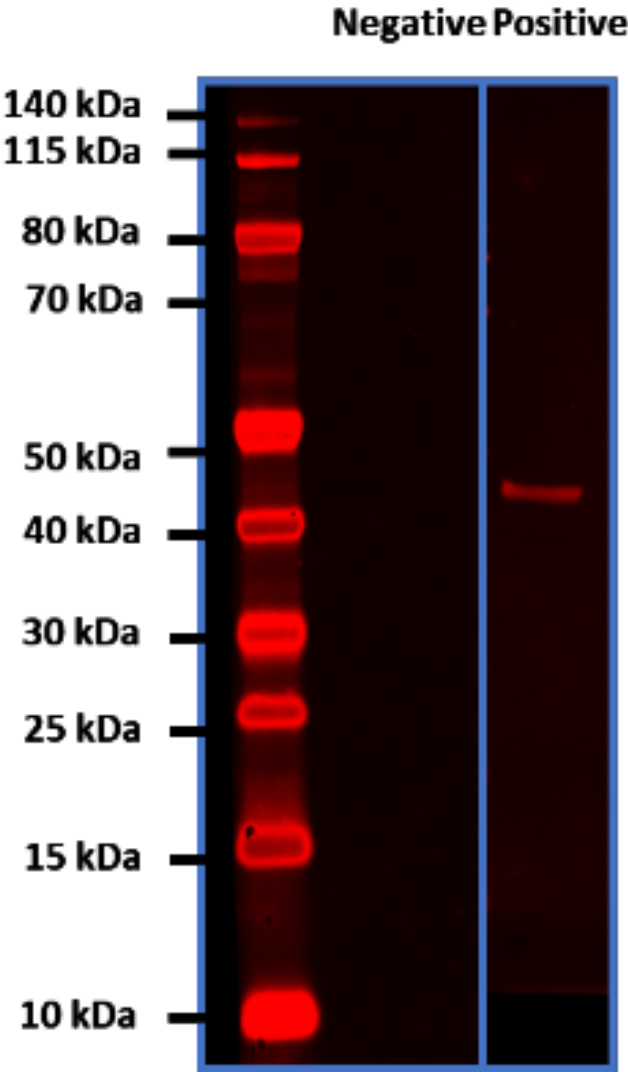

EVIDENCE TIER	Western blot
INSTRUMENT	Azure Sapphire FL
CELL MODEL	HeLa
DETECTED DYES	680
METADATA VALUES	11

STRUCTURED ACQUISITION METADATA / WESTERN BLOT

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Azure Sapphire FL with Customizable Laser and Filter Modules, Enabling UV- NIR and Z-Plane(s)
Scanner	Azure Sapphire FL with Customizable Laser and Filter Modules, Enabling UV- NIR and Z-Plane(s)
Detection mode	Fluorescence
Laser	638nm
Emission Filter	676±37nm
Detector	Avalanche Photodiode
Intensity	8
Pixel size	100 µm
Scan Speed	Medium
Quality	High
Focus	Membrane (0 µm in Z-axis)
Image	Identifyn® LLC

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 680 Affinity Purified Donkey Anti-Mouse IgG (H + L)

Cat ID# - SA 000070

HeLa cells were homogenized using an ultrasonication probe and centrifuged to pellet down the cell debris. The lysate supernatant was mixed with NuPAGE™ LDS Sample Buffer (4X), heated at 80oC for 10 min, and subjected to electrophoresis using NuPAGE™ 4 to 12%, Bis-Tris, 1.0-1.5 mm, Mini Protein Gels in a Mini Gel Tank. The Thermo Fisher's PageRuler™ Prestained Protein Ladder, 10 to 180 kDa, was used as a molecular weight marker.

Post electrophoresis, the proteins were transferred to a polyvinylidene difluoride (PVDF) membrane using iBlot™ 3 Starter Kit, PVDF. The transfer membrane was blocked with Blocker™ Casein for 1 hour and washed 5X with PBS. The blocked membrane was incubated with Actin Monoclonal Antibody (mAbGEa) (MA1-744) for 2 hours, followed by 5X PBS washes. Identifyn® SRM Alexa Fluor™ 680 Affinity Purified Donkey anti-Mouse IgG (H+L) was incubated for 1 hour, followed by washing 5X with PBS. The membrane was dried for 10 minutes at room temperature before imaging.

Scanner = Azure Sapphire FL with Customizable Laser and Filter Modules, Enabling UV- NIR and Z-Plane(s)

Scan Settings

Detection mode = Fluorescence

Laser = 638nm

Emission Filter = 676±37nm

Detector = Avalanche Photodiode

Intensity = 8

Pixel size = 100 µm

Scan Speed = Medium

Quality = High

Focus = Membrane (0 µm in Z-axis)

Post Processing

None

Image: Identifyn® LLC

Copyright 2026 GMD12 LLC.


SOURCE PROVENANCE

Catalog	SA-000070
Stage	Western blot
Instrument	Azure Sapphire FL
Microscope configuration	Azure Sapphire FL with Customizable Laser and Filter Modules, Enabling UV- NIR and Z-Plane(s)

SOURCE PROVENANCE

Structured source metadata values	11
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	7B21728EC75AA21F8B4FC6CA4EFAF2F75030145CCF1CB9870CD85D02928CBC6C
Method PDF SHA-256	67D05FAE2A3F3BC3C1300F4B66D4FDF3E793040043CE065E81DCE837BAEC4BE9

ORIGINAL IMAGE EVIDENCE / WIDEFIELD

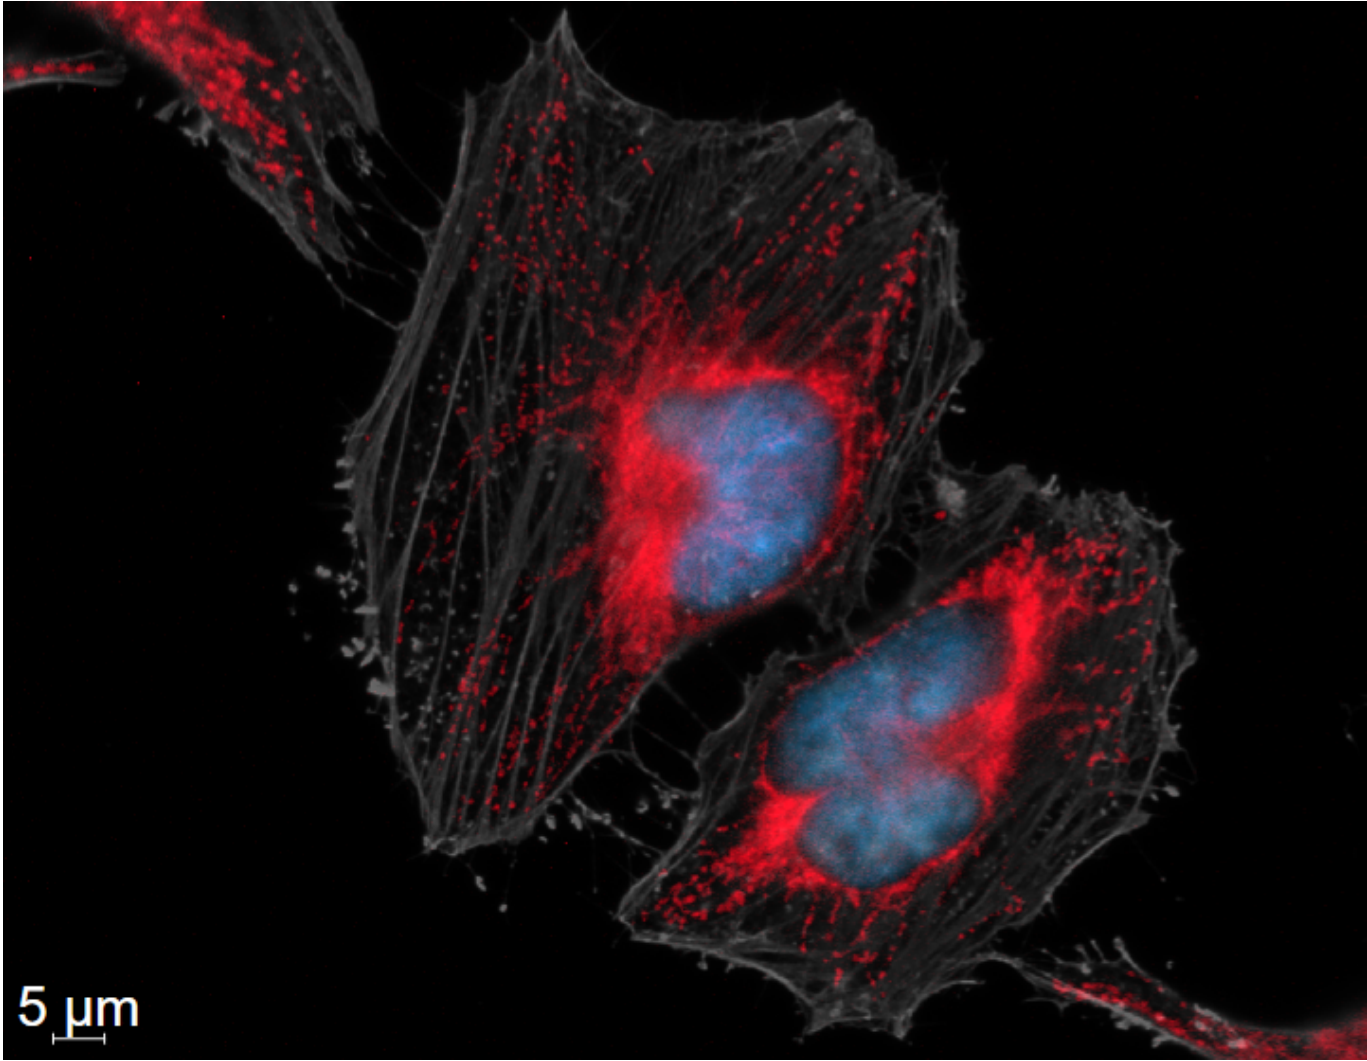

EVIDENCE TIER	Widefield
INSTRUMENT	ZEISS Axio Imager.M1
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 555; 680
METADATA VALUES	38

STRUCTURED ACQUISITION METADATA / WIDEFIELD

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss Axio Imager.M1 Widefield, using a Plan-Apochromat 63x/1.40 Oil M27, Axiocam 705, and X-Cite Xylis Lamp was used with the following parameters for each dye:
Objective	Plan-Apochromat 63x/1.40 Oil M27
Channels	3
Scaling (Per Pixel)	0.102µm X 0.102µm
Image size (Pixels)	1388 X 1040
Image Size (Scaled)	142.10µm X 106.48µm
Bit Depth	12 Bit
Image Center Position	X: 0.00µm, Y: 0.00µm
ROI Center Offset	X: 0.00µm, Y: 0.00µm
Reflector	50 Cy5 4AF532-49014 49 DAPI
Beam Splitter	660 550 395
Filter Excitation Wavelength	625 - 655 515 - 545 335 - 383
Filter Emission Wavelength	665 - 715 555 - 595 420 - 470
Contrast Method	Fluorescence
Light source	X-Cite Xylis Lamp Intensity @30% X-Cite Xylis Lamp Intensity @15%
Exposure Time	400ms 100ms 80ms
Excitation Wavelength	679 553 353
Emission Wavelength	702 568 465
Effective NA	1.4
Imaging Device	Axiocam 705
Camera Adapter	1X
Depth of Focus	1.09µm 0.88µm 0.72µm
Binning Mode	1,1

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 680 Affinity Purified Donkey Anti-Mouse IgG (H + L)

Cat ID# - SA 000070

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit IgG (H + L)

Cat ID# - SA 000035

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher, Fish Serum Blocker cat#37527X3. The first primary antibody, Mitochondria Antibody (MA5-12017), was incubated overnight at 4°C at a dilution of 1:100. Cells were washed 3X in PBS. Identifyn® 680 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000.

The second primary antibody followed this, Actin Recombinant Rabbit Monoclonal Antibody (JF47-01), which was incubated for 1 hour at room temperature at a dilution of 1:250. Cells were washed 3X in PBS. Identifyn® 555 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss Axio Imager.M1 Widefield, using a Plan-Apochromat 63x/1.40 Oil M27, Axiocam 705, and X-Cite Xylis Lamp was used with the following parameters for each dye:

Single Plane (2D)

Channels = 3

Scaling (Per Pixel) = 0.102µm X 0.102µm

Image size (Pixels) = 1388 X 1040

Image Size (Scaled) = 142.10µm X 106.48µm

Bit Depth = 12 Bit

Image Center Position = X: 0.00µm, Y: 0.00µm

ROI Center Offset = X: 0.00µm, Y: 0.00µm

680 -

Reflector = 50 Cy5

Beam Splitter = 660

Filter Excitation Wavelength = 625 - 655

Filter Emission Wavelength = 665 - 715

Contrast Method = Fluorescence

Light source = X-Cite Xylis Lamp Intensity @30%

Exposure Time = 400ms

Excitation Wavelength = 679

Emission Wavelength = 702

Effective NA = 1.4

Imaging Device = Axiocam 705

Camera Adapter = 1X

Depth of Focus = 1.09µm

Binning Mode = 1,1

555 -

Reflector = 4AF532-49014
 Beam Splitter = 550
 Filter Excitation Wavelength = 515 - 545
 Filter Emission Wavelength = 555 - 595
 Contrast Method = Fluorescence
 Light source = X-Cite Xylis Lamp Intensity @30%
 Exposure Time = 100ms
 Excitation Wavelength = 553
 Emission Wavelength = 568
 Effective NA = 1.4
 Imaging Device = Axiocam 705
 Camera Adapter = 1X
 Depth of Focus = 0.88μm
 Binning Mode = 1,1

DAPI -

Reflector = 49 DAPI
 Beam Splitter = 395
 Filter Excitation Wavelength = 335 - 383
 Filter Emission Wavelength = 420 - 470
 Contrast Method = Fluorescence
 Light source = X-Cite Xylis Lamp Intensity @15%
 Exposure Time = 80ms
 Excitation Wavelength = 353
 Emission Wavelength = 465
 Effective NA = 1.4
 Imaging Device = Axiocam 705
 Camera Adapter = 1X
 Depth of Focus = 0.72μm
 Binning Mode = 1,1

Post Processing

Identifyn® SRM Alexa Fluor™ 555 was pseudo-colored in Zen Software from orange, the default color, to white to provide visual contrast between the 555/680 channels.

Image Correction

None

Image by E.F. Simon

Copyright 2026 GMD12 LLC.


SOURCE PROVENANCE

Catalog	SA-000070
---------	-----------

SOURCE PROVENANCE

Stage	Widefield
Instrument	ZEISS Axio Imager.M1
Microscope configuration	Zeiss Axio Imager.M1 Widefield, using a Plan-Apochromat 63x/1.40 Oil M27, AxioCam 705, and X-Cite Xylys Lamp was used with the following parameters for each dye:
Structured source metadata values	38
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	9DA93073445C9FFF2927D0E2EE7145471B46C9DA022828721A11489B08F853D2
Method PDF SHA-256	B2BD3D8258F659C0FAB57BDF235044730442C79A2B152D03DBC2EA27380BD7D4

ORIGINAL IMAGE EVIDENCE / WIDEFIELD SIM - APOTOME

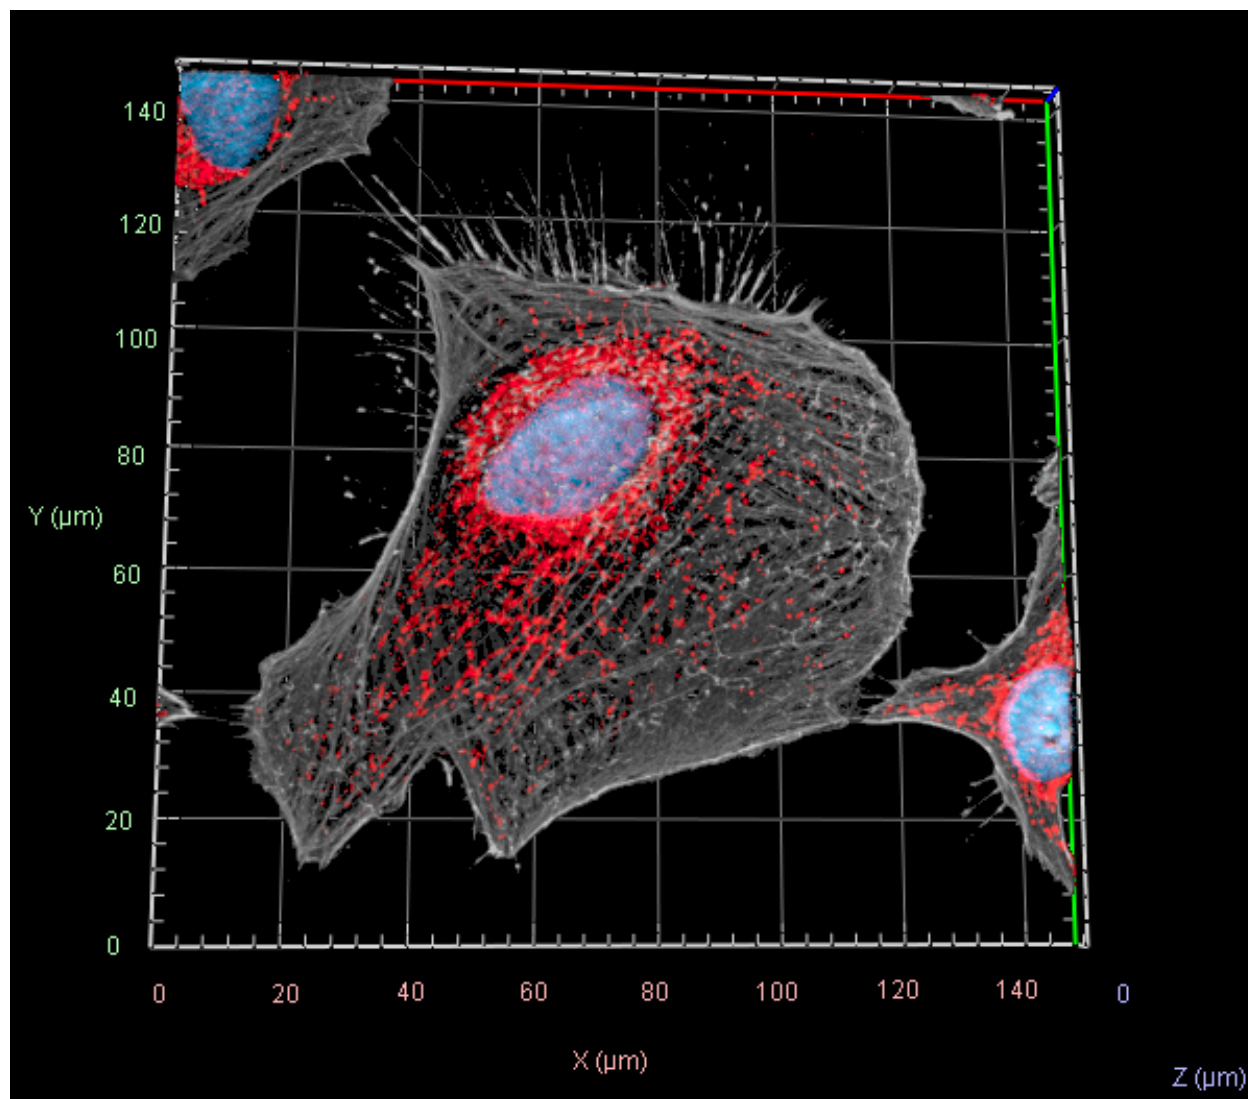

EVIDENCE TIER	Widefield SIM - Apotome
INSTRUMENT	ZEISS Axio Observer.Z1/7 Apotome
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 532; 555; 680
METADATA VALUES	47

STRUCTURED ACQUISITION METADATA / WIDEFIELD SIM - APOTOME

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:
Objective	EC Plan-Neofluar 63X/1.25 oil M27
Z-Stack	29 Slices (5.6µm)
Channels	3
Scaling (Per Pixel)	0.143µm X 0.143µm X 0.200µm
Image Size (Pixels)	1037 X 1005
Image Size (Scaled)	148.14µm X 143.57µm
Bit Depth	14 Bit
Image Center Position	X: 56.60mm, Y: 53.07mm
Stage Position	X: 56.60mm, Y: 53.07mm
ROI Center Offset	X: 1.14, Y: 0.00µm
Reflector	50 Cy5 AF532-49014 49 DAPI
Beam Splitter	660 550 395
Filter Excitation Wavelength	625 - 655 515 - 545 335 - 383
Filter Emission Wavelength	665 - 715 555 - 595 420 - 470
Contrast Method	Fluorescence
Light source	X-Cite Xylis Lamp Intensity @85% X-Cite Xylis Lamp Intensity @25% X-Cite Xylis Lamp Intensity @8%
Exposure Time	380ms 150ms 25ms
Excitation Wavelength	679 553 353
Emission Wavelength	702 568 465
Effective NA	1.25
Imaging Device	Axiocam 807
Camera Adapter	1X
Depth of Focus	1.36µm 1.10µm 0.90µm
Binning Mode	2,2
Apotome SIM Image Processing	Display Mode "Optical Sectioning" - enabled correction selected.
3D Maximum Projection	Precise
Appearance	Threshold 13% (680), Threshold 13% (532), Threshold 13% (DAPI), Ramp 0% all channels, Maximum 100% all channels
Background	Black
Light	Brightness 100%, Enabled Tone Mapping
Projection	View Angle 35°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 680 Affinity Purified Donkey Anti-Mouse IgG (H + L)

Cat ID# - SA 000070

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit IgG (H + L)

Cat ID# - SA 000035

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher, Fish Serum Blocker cat#37527X3. The first primary antibody, Mitochondria Antibody (MA5-12017), was incubated overnight at 4°C at a dilution of 1:100. Cells were washed 3X in PBS. Identifyn® 680 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000.

The second primary antibody followed this, Actin Recombinant Rabbit Monoclonal Antibody (JF47-01), which was incubated for 1 hour at room temperature at a dilution of 1:250. Cells were washed 3X in PBS. Identifyn® 555 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:

Z Stack - (3D)

Z-Stack = 29 Slices (5.6µm)

Channels = 3

Scaling (Per Pixel) = 0.143µm X 0.143µm X 0.200µm

Image Size (Pixels) = 1037 X 1005

Image Size (Scaled) = 148.14µm X 143.57µm

Bit Depth = 14 Bit

Image Center Position = X: 56.60mm, Y: 53.07mm

Stage Position = X: 56.60mm, Y: 53.07mm

ROI Center Offset = X: 1.14, Y: 0.00µm

680 -

Reflector = 50 Cy5
 Beam Splitter = 660
 Filter Excitation Wavelength = 625 - 655
 Filter Emission Wavelength = 665 - 715
 Contrast Method = Fluorescence
 Light source = X-Cite Xylis Lamp Intensity @85%
 Exposure Time = 380ms
 Excitation Wavelength = 679
 Emission Wavelength = 702
 Effective NA = 1.25
 Imaging Device = Axiocam 807
 Camera Adapter = 1X
 Depth of Focus = 1.36µm
 Binning Mode = 2,2

555 -

Reflector = AF532-49014
 Beam Splitter = 550
 Filter Excitation Wavelength = 515 - 545
 Filter Emission Wavelength = 555 - 595
 Contrast Method = Fluorescence
 Light source = X-Cite Xylis Lamp Intensity @25%
 Exposure Time = 150ms
 Excitation Wavelength = 553
 Emission Wavelength = 568
 Effective NA = 1.25
 Imaging Device = Axiocam 807
 Camera Adapter = 1X
 Depth of Focus = 1.10µm
 Binning Mode = 2,2

DAPI -

Reflector = 49 DAPI
 Beam Splitter = 395
 Filter Excitation Wavelength = 335 - 383
 Filter Emission Wavelength = 420 - 470
 Contrast Method = Fluorescence
 Light source = X-Cite Xylis Lamp Intensity @8%
 Exposure Time = 25ms
 Excitation Wavelength = 353
 Emission Wavelength = 465
 Effective NA = 1.25
 Imaging Device = Axiocam 807
 Camera Adapter = 1X
 Depth of Focus = 0.90µm
 Binning Mode = 2,2

Post Processing - SIM Processing

Apotome SIM Image Processing = Display Mode “Optical Sectioning” - enabled correction selected.

Normalization, Phase Correction, Fourier Filter, and Deconvolution were NOT used.

3D Image Processing

3D Maximum Projection = Precise

Appearance = Threshold 13% (680), Threshold 13% (532), Threshold 13% (DAPI), Ramp 0% all channels, Maximum 100% all channels

Background = Black

Light = Brightness 100%, Enabled Tone Mapping

Projection = View Angle 35°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

Image Corrections

Identifyn® SRM Alexa Fluor™ 555 was pseudo-colored in Zen Software from orange, the default color, to white to provide visual contrast between the 405/680 channels.


Image by E.F. Simon

Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE

Catalog	SA-000070
Stage	Widefield SIM - Apotome
Instrument	ZEISS Axio Observer.Z1/7 Apotome
Microscope configuration	Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:
Structured source metadata values	47
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	34C357D961D635DB5E8CEFF91723A1F60DB3CC70300C72CE3D1A00420BEFB5A8
Method PDF SHA-256	963A3D36CC3A6727B5F4421D59FFE5F16C63D2391FD196B077BA222A32AD7F11

ORIGINAL IMAGE EVIDENCE / CONFOCAL

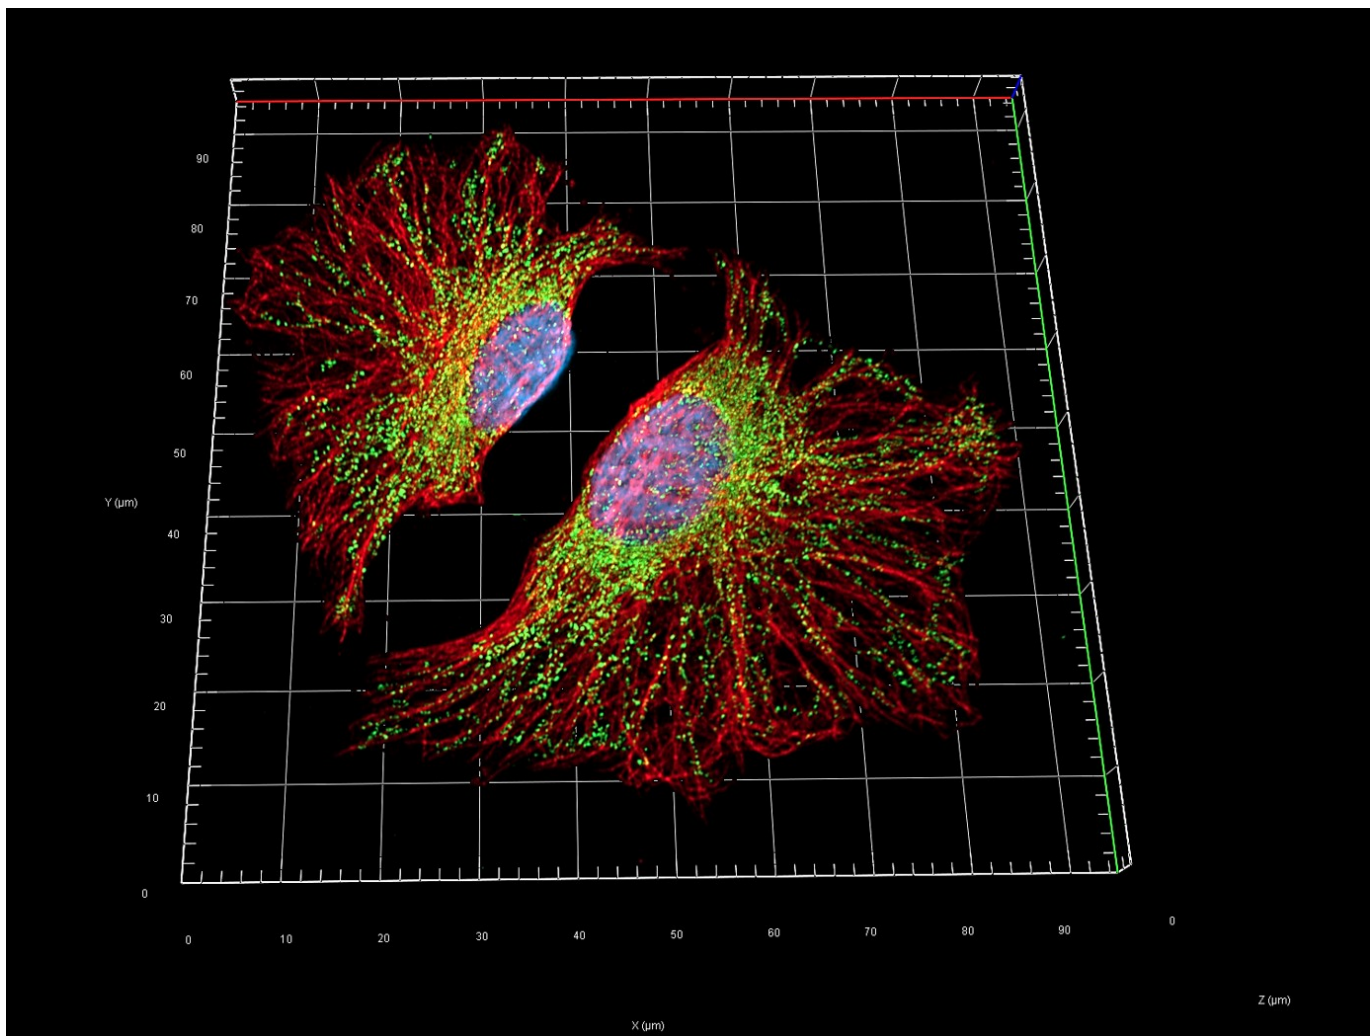

EVIDENCE TIER	Confocal
INSTRUMENT	ZEISS LSM 980
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 488; 532; 680
METADATA VALUES	57

STRUCTURED ACQUISITION METADATA / CONFOCAL

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss LSM 980 Confocal with NIR Detection, Axio Observer.Z1/7, using a Plan-Apochromat 63X/1.40 oil DIC M27, was used with the following parameters for each dye:
Objective	Plan-Apochromat 63X/1.40 oil DIC M27
Z-Stack	62Slices (4.27µm)
Channels	3
Scaling (Per Pixel)	0.059µm X 0.059µm X 0.070µm
Image Size (Pixels)	1612 X 1612
Image Size (Scaled)	94.79µm X 94.79µm
Bit Depth	16 Bit
Image Center Position	X: 71.43mm, Y: 52.11mm
Stage Position	X: 71.43mm, Y: 52.11mm
ROI Center Offset	X: 0.00µm, Y: 0.00µm
Reflector	None
Contrast Method	Fluorescence
Pinhole	1.00AU / 67µm 1.00AU / 49µm 1.00 AU / 42µm
LMS MBS	MBS 488/639, 405/730
LSM SBS	SBS SP 615 Mirror
Laser Wavelength	639nm @0.3% 488nm @0.2% 405nm @0.2%
Laser Blanking	Enabled
Scan Mode	Frame
Scan Zoom	1.4 1.1
Rotation	0°
Sampling	1.20
Pixel Time	0.24µs
Frame Time	6.04s
LSM Scan Speed	11
Scan Direction	Bidirectional
Line Step	1
Averaging	8
Excitation Wavelength	679 493 353
Emission Wavelength	702 517 465
Effective NA	1.4
Detection Wavelength	674 - 702 479 - 540 410 - 469
Imaging Device	GaAsP-Pmt 3 GaAsP-PMT 3

FIELD	SOURCE-DOCUMENTED VALUE
Detector Type	GaAsP-PMT
Detector Gain	600 V 500 V
Detector Offset	0
Detector Digital Gain	1.0
LSM Plus Mode	7.7 (3D, Auto) 7.3 (3D, Auto) 7.2 (3D, Auto)
3D Maximum Projection	Precise
Appearance	Threshold 1% all channels, Ramp 0% all channels, Maximum 100% all channels.
Background	Black
Light	Brightness100%, Tone Mapping NOT Enabled
Projection	View Angle 35°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 680 Affinity Purified Donkey Anti-Mouse IgG (H + L)

Cat ID# - SA 000070

Identifyn® SRM Alexa Fluor™ 488 Affinity Purified Goat Anti-Rabbit, IgG (H + L)

Cat ID# - SA 000058

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher, Fish Serum Blocker cat#37527X3. The first primary antibody, Alpha Tubulin Monoclonal Antibody (DM1A), was incubated overnight at 4°C at a dilution of 1:100. Cells were washed 3X in PBS. Identifyn® 680 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000.

The second primary antibody followed this, Mitochondria Rabbit Recombinant Antibody (MTC02,2860R), which was incubated for 1 hour at room temperature at a dilution of 1:250. Cells were washed 3X in PBS. Identifyn® 532 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss LSM 980 Confocal with NIR Detection, Axio Observer.Z1/7, using a Plan-Apochromat 63X/1.40 oil DIC M27, was used with the following parameters for each dye:

Z Stack - (3D)

Z-Stack = 62Slices (4.27µm)

Channels = 3

Scaling (Per Pixel) = 0.059µm X 0.059µm X 0.070µm

Image Size (Pixels) = 1612 X 1612

Image Size (Scaled) = 94.79µm X 94.79µm

Bit Depth = 16 Bit

Image Center Position = X: 71.43mm, Y: 52.11mm

Stage Position = X: 71.43mm, Y: 52.11mm

ROI Center Offset = X: 0.00µm, Y: 0.00µm

680 -

Reflector = None
Contrast Method = Fluorescence
Pinhole = 1.00AU / 67µm
LMS MBS = MBS 488/639, 405/730
LSM SBS = SBS SP 615
Laser Wavelength = 639nm @0.3%
Laser Blanking = Enabled
Scan Mode = Frame
Scan Zoom = 1.4
Rotation = 0°
Sampling = 1.20
Pixel Time = 0.24µs
Frame Time = 6.04s
LSM Scan Speed = 11
Scan Direction = Bidirectional
Line Step = 1
Averaging = 8
Excitation Wavelength = 679
Emission Wavelength = 702
Effective NA = 1.4
Detection Wavelength = 674 - 702
Imaging Device = GaAsP-Pmt 3
Detector Type = GaAsP-PMT
Detector Gain = 600 V
Detector Offset = 0
Detector Digital Gain = 1.0
LSM Plus Mode = 7.7 (3D, Auto)

532 -

Reflector = None
 Contrast Method = Fluorescence
 Pinhole = 1.00AU / 49µm
 LMS MBS = MBS 488/639, 405/730
 LSM SBS = Mirror
 Laser Wavelength = 488nm @0.2%
 Laser Blanking = Enabled
 Scan Mode = Frame
 Scan Zoom = 1.1
 Rotation = 0°
 Sampling = 1.20
 Pixel Time = 0.24µs
 Frame Time = 6.04s
 LSM Scan Speed = 11
 Scan Direction = Bidirectional
 Line Step = 1
 Averaging = 8
 Excitation Wavelength = 493
 Emission Wavelength = 517
 Effective NA = 1.4
 Detection Wavelength = 479 - 540
 Imaging Device = GaAsP-Pmt 3
 Detector Type = GaAsP-PMT
 Detector Gain = 500 V
 Detector Offset = 0
 Detector Digital Gain = 1.0
 LSM Plus Mode = 7.3 (3D, Auto)

DAPI -

Reflector - None
 Contrast Method - Fluorescence
 Pinhole = 1.00 AU / 42µm
 LMS MBS = MBS 488/639, 405/730
 LSM SBS = Mirror
 Laser Wavelength = 405nm @0.2%
 Laser Blanking = Enabled
 Scan Mode = Frame
 Scan Zoom = 1.4
 Rotation = 0°
 Sampling = 1.20
 Pixel Time = 0.24µs
 Frame Time = 6.04s
 LSM Scan Speed = 11
 Scan Direction = Bidirectional
 Line Step = 1
 Averaging = 8
 Excitation Wavelength = 353
 Emission Wavelength = 465
 Effective NA = 1.4
 Detection Wavelength = 410 - 469
 Imaging Device = GaAsP-PMT 3
 Detector Type = GaAsP-PMT
 Detector Gain = 500 V
 Detector Offset = 0
 Detector Digital Gain = 1.0
 LSM Plus Mode = 7.2 (3D, Auto)

3D Image Processing

3D Maximum Projection = Precise
 Appearance = Threshold 1% all channels, Ramp 0% all channels, Maximum 100% all channels.
 Background = Black
 Light = Brightness100%, Tone Mapping NOT Enabled
 Projection = View Angle 35°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

Image Corrections

None


Image by J.K. Bennett

Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE

Catalog	SA-000070
Stage	Confocal
Instrument	ZEISS LSM 980
Microscope configuration	Zeiss LSM 980 Confocal with NIR Detection, Axio Observer.Z1/7, using a Plan-Apochromat 63X/1.40 oil DIC M27, was used with the following parameters for each dye:
Structured source metadata values	57
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	8C727DD806A86FF9BD71A2306F2E10E717F657D9CB157E82996E77B85C3AF687
Method PDF SHA-256	44392DC0E3F17868659C379F84F81BB1CCEBFB82BBB6AF39FF6128D23FBC57C3

ORIGINAL IMAGE EVIDENCE / AIRYSCAN

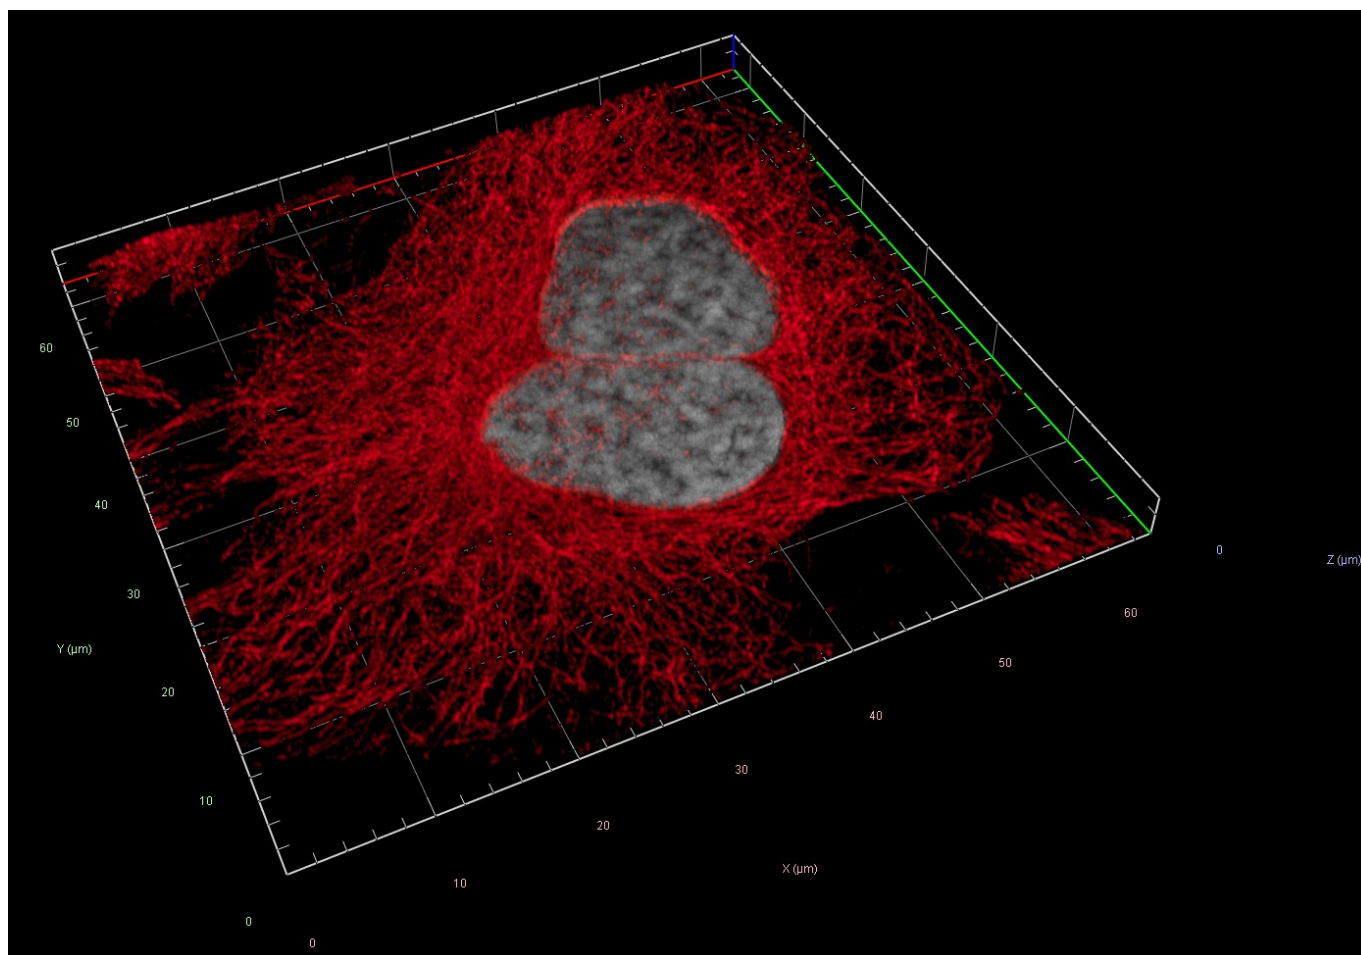

EVIDENCE TIER	Airyscan
INSTRUMENT	ZEISS LSM 980
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 488; 680
METADATA VALUES	47

STRUCTURED ACQUISITION METADATA / AIRYSCAN

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss LSM 980 Confocal with NIR Detection, Axio Observer.Z1/7, using a Plan-Apochromat 63X/1.40 oil DIC M27, was used with the following parameters for each dye:
Objective	Plan-Apochromat 63X/1.40 oil DIC M27
Z-Stack	73 Slices (3.60µm)
Channels	2
Scaling (Per Pixel)	0.03530 µm X 0.03530 µm X 0.05000 µm
Image Size (Pixels)	1793 X 1793
Image Size (Scaled)	63.29µm X 63.29µm
Bit Depth	16 Bit
Image Center Position	X: 69.69mm, Y: 45.79mm
Stage Position	X: 69.69mm, Y: 45.79mm
ROI Center Offset	X: 0.00µm, Y: 0.00µm
Reflector	None
Contrast Method	Fluorescence
Pinhole	5.00AU / 328µm 5.46AU / 235µm
LMS MBS	Plate MBS 488/639 MBS 405/730
LMS SBS	SBS LP 640 SBS SP 505
Laser Wavelength	639nm @0.2% 405nm @0.2%
Laser Blanking	Enabled
Scan Mode	Frame
Scan Zoom	2.1
Rotation	0°
Sampling	2.00
Pixel Time	1.15µs
Frame Time	8.93s
LSM Scan Speed	6
Scan Direction	Bidirectional
Line Step	1
Excitation Wavelength	679 353
Emission Wavelength	702 465
Effective NA	1.4
Detection Wavelength	643 - 735 350 - 499
Imaging Device	Airyscan
Detector Type	GaAsP-PMT

FIELD	SOURCE-DOCUMENTED VALUE
Detector Gain	800 V
Detector Offset	0
Detector Digital Gain	1.0
AiryScan Mode	Super Resolution 9.5 (3D, Auto) Super Resolution 7.8 (3D, Auto)
3D Maximum Projection	Precise
Appearance	Threshold 1% (680), Threshold 1% (DAPI), Ramp 0% (680), Ramp 1% (DAPI), Maximum 100% all channels
Background	Black
Light	Brightness 100%, Enabled Tone Mapping
Projection	View Angle 35°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 680 Affinity Purified Donkey Anti-Mouse IgG (H + L)

Cat ID# - SA 000070

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher, Fish Serum Blocker cat#37527X3. The first primary antibody, Alpha Tubulin Monoclonal Antibody (DM1A), was incubated overnight at 4°C at a dilution of 1:100. Cells were washed 3X in PBS. Identifyn® 680 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss LSM 980 Confocal with NIR Detection, Axio Observer.Z1/7, using a Plan-Apochromat 63X/1.40 oil DIC M27, was used with the following parameters for each dye:

Z Stack - (3D)

Z-Stack =73 Slices (3.60µm)

Channels = 2

Scaling (Per Pixel) = 35.30nm X 35.30nm X 50.00nm

Image Size (Pixels) = 1793 X 1793

Image Size (Scaled) = 63.29µm X 63.29µm

Bit Depth = 16 Bit

Image Center Position = X: 69.69mm, Y: 45.79mm

Stage Position =X: 69.69mm, Y: 45.79mm

ROI Center Offset = X: 0.00µm, Y: 0.00µm

680 -

Reflector = None
 Contrast Method = Fluorescence
 Pinhole = 5.00AU / 328µm
 LMS MBS = Plate MBS 488/639 MBS 405/730
 LMS SBS = SBS LP 640
 Laser Wavelength = 639nm @0.2%
 Laser Blanking = Enabled
 Scan Mode = Frame
 Scan Zoom = 2.1
 Rotation = 0°
 Sampling = 2.00
 Pixel Time = 1.15µs
 Frame Time = 8.93s
 LSM Scan Speed = 6
 Scan Direction = Bidirectional
 Line Step = 1
 Averaging - 2
 Excitation Wavelength = 679
 Emission Wavelength = 702
 Effective NA = 1.4
 Detection Wavelength = 643 - 735
 Imaging Device = Airyscan
 Detector Type = GaAsP-PMT
 Detector Gain = 800 V
 Detector Offset = 0
 Detector Digital Gain = 1.0
 AiryScan Mode = Super Resolution 9.5 (3D, Auto)

DAPI -

Reflector = None
 Contrast Method = Fluorescence
 Pinhole = 5.46AU / 235µm
 LMS MBS = Plate MBS 488/639 MBS 405/730
 LMS SBS = SBS SP 505
 Laser Wavelength = 405nm @0.2%
 Laser Blanking = Enabled
 Scan Mode = Frame
 Scan Zoom = 2.1
 Rotation = 0°
 Sampling = 2.00
 Pixel Time = 1.15µs
 Frame Time = 8.93s
 LSM Scan Speed = 6
 Scan Direction = Bidirectional
 Line Step = 1
 Averaging - 2
 Excitation Wavelength = 353
 Emission Wavelength = 465
 Effective NA = 1.4
 Detection Wavelength = 350 - 499
 Imaging Device = Airyscan
 Detector Type = GaAsP-PMT
 Detector Gain = 800 V
 Detector Offset = 0
 Detector Digital Gain = 1.0
 AiryScan Mode = Super Resolution 7.8 (3D, Auto)

3D Image Processing

3D Maximum Projection = Precise
 Appearance = Threshold 1% (680), Threshold 1% (DAPI), Ramp 0% (680), Ramp 1% (DAPI), Maximum 100% all channels
 Background = Black
 Light = Brightness 100%, Enabled Tone Mapping
 Projection = View Angle 35°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

Image Corrections

DAPI was pseudo-colored in Zen Software from blue, the default color, to dark grey to provide visual contrast between the 680 and DAPI channels.


Image by J. K. Bennett

Copyright 2026 GMD12 LLC.
 Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE

Catalog	SA-000070
Stage	Airyscan
Instrument	ZEISS LSM 980
Microscope configuration	Zeiss LSM 980 Confocal with NIR Detection, Axio Observer.Z1/7, using a Plan-Apochromat 63X/1.40 oil DIC M27, was used with the following parameters for each dye:
Structured source metadata values	47
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	06799399CD922DE6BD440D91D3486B0C32851AF22F0D3E634993F901C61E612A
Method PDF SHA-256	06D1F2085C004604D842085FA79B66510C7DF97C328F402E3C06D1F7AFD75C29

ORIGINAL IMAGE EVIDENCE / SIM

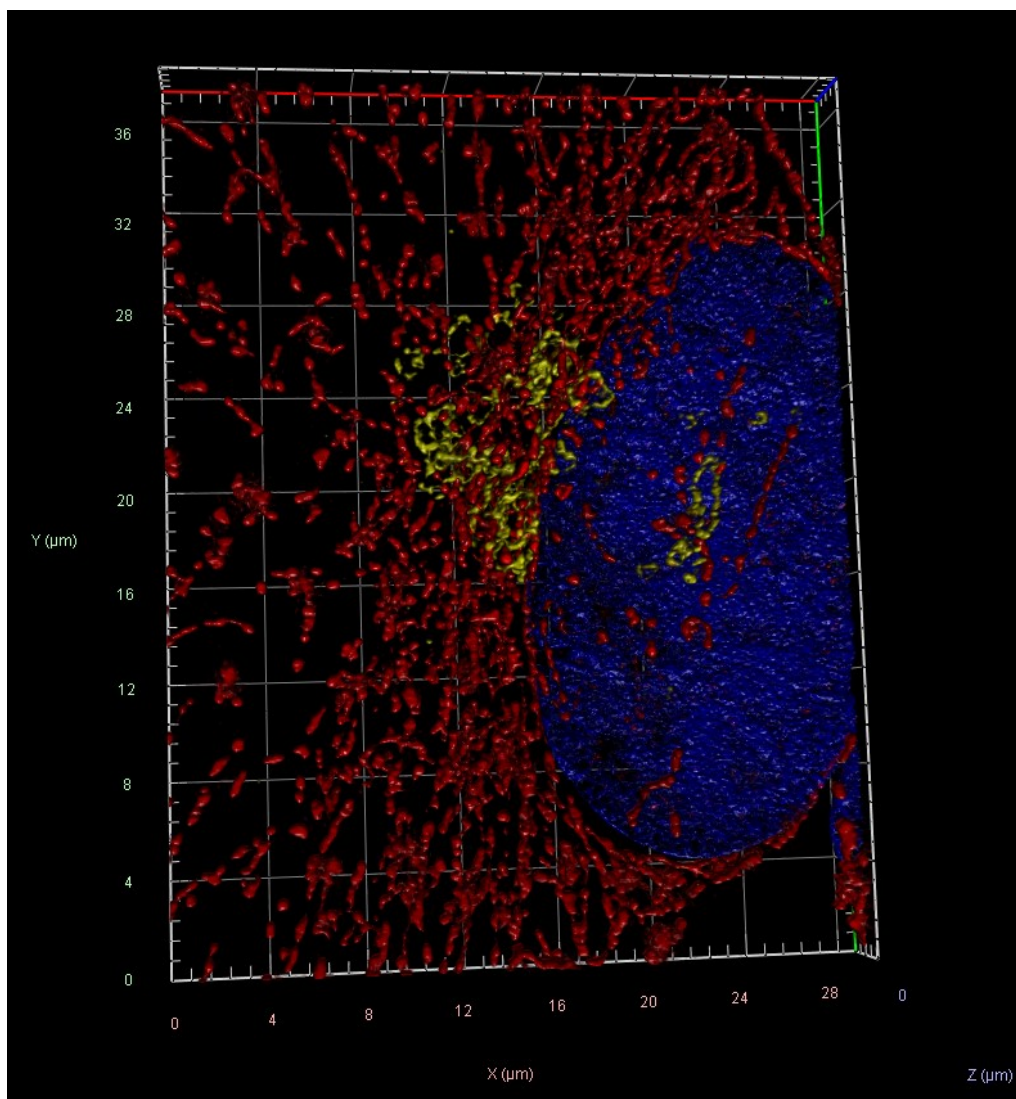

EVIDENCE TIER	SIM
INSTRUMENT	ZEISS Elyra
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 488; 555; 680
METADATA VALUES	59

STRUCTURED ACQUISITION METADATA / SIM

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss Elyra 5 Lattice SIM, AxioObserver.Z1/ 7 using Plan-Apochromat 63X/1.40 oil DIC M27, 1X Tubelens, was used with the following parameters for each dye:
Objective	Plan-Apochromat 63X/1.40 oil DIC M27
Z-Stack	68 Slices (3.35µm)
Channels	3
Scaling (Per Pixel)	0.01320 µm X 0.01320 µm X 0.05000 µm
Image Size (Pixels)	2180 X 2828
Image Size (Scaled)	28.77µm X 37.32µm
Bit Depth	16 Bit
Image Center Position	X: 59.25mm, Y: 34.77mm
Stage Position	X: 59.25mm, Y: 34.77mm
ROI Center Offset	X: 0.00µm, Y: 0.00µm
Reflectors	SR HE LBF 405/488/561/642
Beam Splitter	405, 488, 561, 642
Filter Excitation Wavelength	200 - 405, 200 - 488, 200 - 561, 200 - 642
Filter Emission Wavelength	419 - 470, 503 - 546, 576 - 617, 657 - 800
Contrast Method	Fluorescence
Illumination Wavelength	640 561 405
Channel Name	T1-Axiocam 820 -SR T2-Axiocam 820 #2-SR T3-Axiocam 820 #2 -SR
Excitation Wavelength	640 561 405
Emission Wavelength	729 597 445
Effective NA	1.4
Detection Wavelength	419-470, 503-546, 576-617, 657-800
Imaging Device	Axiocam 820 Axiocam 820 #2
Camera Adapter	1X
Exposure Time	150ms 100ms 50ms
Depth of Focus	1.13µm 0.92µm 0.69µm
Binning Mode	2,2
Laser Wavelength	640nm @8.0% 561nm @1.00% 405nm @10%
Frame Time	1.98s 1.33s 676.00ms
Scan Direction	Unidirectional
Result Sampling	4
Process Sampling	N/A
Algorithm	SIM

FIELD	SOURCE-DOCUMENTED VALUE
SIM Settings	Standard
Auto Sharpness	On
Sharpness	9.8664 (680), 10.2339 (555), 8.7886 (DAPI)
Fitting	Fast Fit
Histogram	Scale to Min/Max
Baseline	Cut
3D Volume Projection	Precise
Appearance	Threshold 2% (680), Threshold 2% (555), Threshold 2% (DAPI), Ramp 0% all channels, Maximum 100% all channels
Background	Black
Light	Brightness 114%, Azimuth 69°, Elongation -80°, Enabled Directional Lighting, Enabled Tone Mapping
Projection	View Angle 35°, Scale Z 86%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 680 Affinity Purified Donkey Anti-Mouse IgG (H + L)

Cat ID# - SA 000070

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit IgG (H + L)

Cat ID# - SA 000035

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher, Fish Serum Blocker cat#37527X3. The first primary antibody, Golgi GOLPH2 Polyclonal Antibody, was incubated overnight at 4°C at a dilution of 1:100. Cells were washed 3X in PBS. Identifyn® 555 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000.

The second primary antibody followed this, Mitochondria Antibody (MA5-12017), which was incubated for 1 hour at room temperature at a dilution of 1:250. Cells were washed 3X in PBS. Identifyn® 680 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss Elyra 5 Lattice SIM, AxioObserver.Z1/ 7 using Plan-Apochromat 63X/1.40 oil DIC M27, 1X Tubelens, was used with the following parameters for each dye:

Z Stack - (3D)

Z-Stack = 68 Slices (3.35µm)

Channels = 3

Scaling (Per Pixel) = 13.20nm X 13.20nm X 50.00nm

Image Size (Pixels) = 2180 X 2828

Image Size (Scaled) = 28.77µm X 37.32µm

Bit Depth = 16 Bit

Image Center Position = X: 59.25mm, Y: 34.77mm

Stage Position = X: 59.25mm, Y: 34.77mm

ROI Center Offset = X: 0.00µm, Y: 0.00µm

680 -

Reflectors = SR HE LBF 405/488/561/642
 Beam Splitter = 405, 488, 561, 642
 Filter Excitation Wavelength = 200 - 405, 200 - 488, 200 - 561, 200 - 642
 Filter Emission Wavelength = 419 - 470, 503 - 546, 576 - 617, 657 - 800
 Contrast Method = Fluorescence
 Illumination Wavelength = 640
 Channel Name = T1-Axiocam 820 -SR
 Excitation Wavelength = 640
 Emission Wavelength = 729
 Effective NA = 1.4
 Detection Wavelength = 419-470, 503-546, 576-617, 657-800
 Imaging Device = Axiocam 820
 Camera Adapter = 1X
 Exposure Time = 150ms
 Depth of Focus = 1.13µm
 Binning Mode = 2,2
 Laser Wavelength = 640nm @8.0%
 Frame Time = 1.98s
 Scan Direction = Unidirectional
 Grating 36.5µm grating

555 -

Reflectors = SR HE LBF 405/488/561/642
 Beam Splitter = 405, 488, 561, 642
 Filter Excitation Wavelength = 200 - 405, 200 - 488, 200 - 561, 200 - 642
 Filter Emission Wavelength = 419 - 470, 503 - 546, 576 - 617, 657 - 800
 Contrast Method = Fluorescence
 Illumination Wavelength = 561
 Channel Name = T2-Axiocam 820 #2-SR
 Excitation Wavelength = 561
 Emission Wavelength = 597
 Effective NA = 1.4
 Detection Wavelength = 419-470, 503-546, 576-617, 657-800
 Imaging Device = Axiocam 820 #2
 Camera Adapter = 1X
 Exposure Time = 100ms
 Depth of Focus = 0.92µm
 Binning Mode = 2,2
 Laser Wavelength = 561nm @1.00%
 Frame Time = 1.33s
 Scan Direction = Unidirectional
 Grating 32.0µm grating

DAPI -

Reflectors = SR HE LBF 405/488/561/642
 Beam Splitter = 405, 488, 561, 642
 Filter Excitation Wavelength = 200 - 405, 200 - 488, 200 - 561, 200 - 642
 Filter Emission Wavelength = 419 - 470, 503 - 546, 576 - 617, 657 - 800
 Contrast Method = Fluorescence
 Illumination Wavelength = 405
 Channel Name = T3-Axiocam 820 #2 -SR
 Excitation Wavelength = 405
 Emission Wavelength = 445
 Effective NA = 1.4
 Detection Wavelength = 419-470, 503-546, 576-617, 657-800
 Imaging Device = Axiocam 820 #2
 Camera Adapter = 1X
 Exposure Time = 50ms
 Depth of Focus = 0.69µm
 Binning Mode = 2,2
 Laser Wavelength = 405nm @10%
 Frame Time = 676.00ms
 Scan Direction = Unidirectional
 Grating 36.5µm grating

Post Processing - SIM Processing

Processing Dimension - 3D
 Result Sampling = 4
 Process Sampling = N/A
 Channels = 3
 Algorithm = SIM
 SIM Settings = Standard
 Auto Sharpness = On
 Sharpness = 9.8664 (680), 10.2339 (555), 8.7886 (DAPI)
 Fitting = Fast Fit
 Histogram = Scale to Min/Max
 Baseline = Cut

3D Image Processing

3D Volume Projection = Precise
 Appearance = Threshold 2% (680), Threshold 2% (555), Threshold 2% (DAPI), Ramp 0% all channels, Maximum 100% all channels
 Background = Black
 Light = Brightness 114%, Azimuth 69°, Elongation -80°, Enabled Directional Lighting, Enabled Tone Mapping
 Projection = View Angle 35°, Scale Z 86%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

Image Corrections

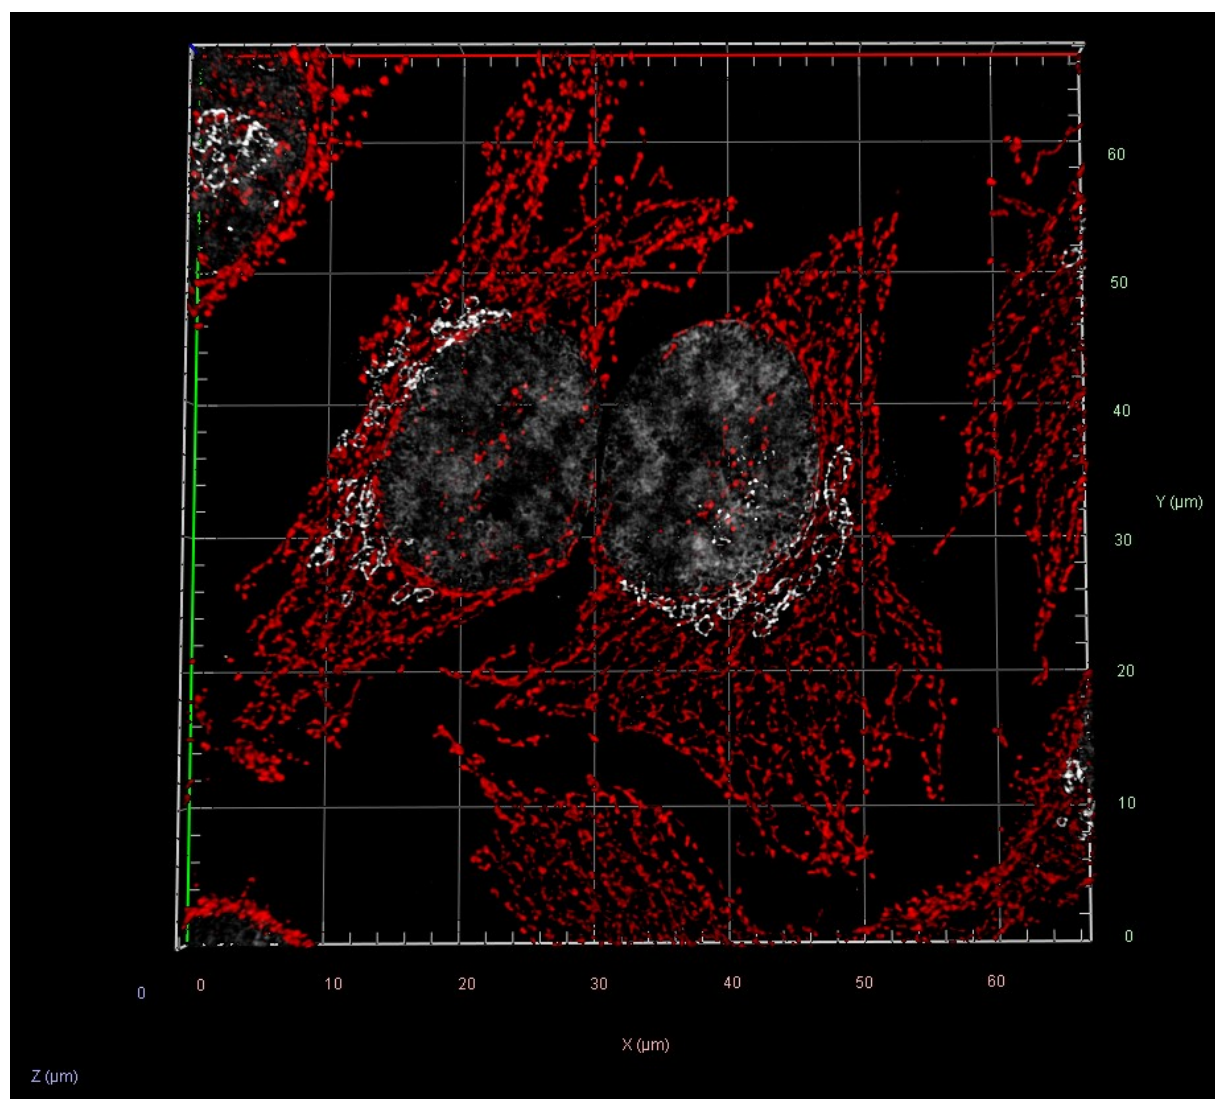
None

Image by P. Raut

Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE

Catalog	SA-000070
Stage	SIM
Instrument	ZEISS Elyra
Microscope configuration	Zeiss Elyra 5 Lattice SIM, AxioObserver.Z1/ 7 using Plan-Apochromat 63X/1.40 oil DIC M27, 1X Tubelens, was used with the following parameters for each dye:
Structured source metadata values	59
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	A8123C927F3A9496748AB97E6D212EB7130324B2D6BCAB78DB0B7A3FA5719A69
Method PDF SHA-256	C31517941F2E01E1AEDC2859B2D6D4AEA97D2A9FD083AF849E737C3F4E5DC083

ORIGINAL IMAGE EVIDENCE / SIM²

EVIDENCE TIER	SIM ²
INSTRUMENT	ZEISS Elyra
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 488; 555; 647; 680
METADATA VALUES	63

STRUCTURED ACQUISITION METADATA / SIM²

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss Elyra 5 Lattice SIM, AxioObserver.Z1/ 7 using Plan-Apochromat 63X/1.40 oil DIC M27, 1X Tubelens, was used with the following parameters for each dye:
Objective	Plan-Apochromat 63X/1.40 oil DIC M27
Z-Stack	54 Slices (2.65µm)
Channels	3
Scaling (Per Pixel)	0.01320 µm X 0.01320 µm X 0.05000 µm
Image Size (Pixels)	5056 X 5056
Image Size (Scaled)	66.72µm X 66.72µm
Bit Depth	16 Bit
Image Center Position	X: 57.11mm, Y: 34.96mm
Stage Position	X: 57.11mm, Y: 34.96mm
ROI Center Offset	X: 0.00µm, Y: 0.00µm
Reflectors	SR HE LBF 405/488/561/642
Beam Splitter	405, 488, 561, 642
Filter Excitation Wavelength	200 - 405, 200 - 488, 200 - 561, 200 - 642
Filter Emission Wavelength	419 - 470, 503 - 546, 576 - 617, 657 - 800
Contrast Method	Fluorescence
Illumination Wavelength	640 561 405
Channel Name	T1-Axiocam 820 -SR T2-Axiocam 820 #2-SR T3-Axiocam 820 #2 -SR
Excitation Wavelength	640 561 405
Emission Wavelength	729 597 445
Effective NA	1.4
Detection Wavelength	419-470, 503-546, 576-617, 657-800
Imaging Device	Axiocam 820 Axiocam 820 #2
Camera Adapter	1X
Exposure Time	150ms 100ms 50ms
Depth of Focus	1.13µm 0.92µm 0.69µm
Binning Mode	2,2
Laser Wavelength	640nm @8.0% 561nm @1.00% 640nm @10%
Frame Time	1.98s 1.33s 676.00ms
Scan Direction	Unidirectional
Result Sampling	4
Process Sampling	4
Algorithm	SIM2

FIELD	SOURCE-DOCUMENTED VALUE
SIM Settings	Standard
Auto Sharpness	On
Sharpness	8.8948 (690), 9.4656 (555), 7.8076 (DAPI)
Order Combination	Weiner filter
Regularization	None
Regularization Weight	0.0000
Iterations	3
Filter	No Filter
Fitting	Fast Fit
Histogram	Scale to Min/Max
3D Maximum Projection	Precise
Appearance	Threshold 1% (647), Threshold 1% (555), Threshold 1% (DAPI), Ramp 0% all channels, Maximum 100% all channels
Background	Black
Light	Brightness 125%, Enabled Tone Mapping
Projection	View Angle 35°, Scale Z 275%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 680 Affinity Purified Donkey Anti-Mouse IgG (H + L)

Cat ID# - SA 000070

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit IgG (H + L)

Cat ID# - SA 000035

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher, Fish Serum Blocker cat#37527X3. The first primary antibody, Golgi GOLPH2 Polyclonal Antibody, was incubated overnight at 4°C at a dilution of 1:100. Cells were washed 3X in PBS. Identifyn® 555 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000.

The second primary antibody followed this, Mitochondria Antibody (MA5-12017), which was incubated for 1 hour at room temperature at a dilution of 1:250. Cells were washed 3X in PBS. Identifyn® 680 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss Elyra 5 Lattice SIM, AxioObserver.Z1/ 7 using Plan-Apochromat 63X/1.40 oil DIC M27, 1X Tubelens, was used with the following parameters for each dye:

Z Stack - (3D)

Z-Stack = 54 Slices (2.65µm)

Channels = 3

Scaling (Per Pixel) = 13.20nm X 13.20nm X 50.00nm

Image Size (Pixels) = 5056 X 5056

Image Size (Scaled) = 66.72µm X 66.72µm

Bit Depth = 16 Bit

Image Center Position = X: 57.11mm, Y: 34.96mm

Stage Position = X: 57.11mm, Y: 34.96mm

ROI Center Offset = X: 0.00µm, Y: 0.00µm

680 -

Reflectors = SR HE LBF 405/488/561/642
 Beam Splitter = 405, 488, 561, 642
 Filter Excitation Wavelength = 200 - 405, 200 - 488, 200 - 561, 200 - 642
 Filter Emission Wavelength = 419 - 470, 503 - 546, 576 - 617, 657 - 800
 Contrast Method = Fluorescence
 Illumination Wavelength = 640
 Channel Name = T1-Axiocam 820 -SR
 Excitation Wavelength = 640
 Emission Wavelength = 729
 Effective NA = 1.4
 Detection Wavelength = 419-470, 503-546, 576-617, 657-800
 Imaging Device = Axiocam 820
 Camera Adapter = 1X
 Exposure Time = 150ms
 Depth of Focus = 1.13µm
 Binning Mode = 2,2
 Laser Wavelength = 640nm @8.0%
 Frame Time = 1.98s
 Scan Direction = Unidirectional
 Grating 36.5µm grating

555 -

Reflectors = SR HE LBF 405/488/561/642
 Beam Splitter = 405, 488, 561, 642
 Filter Excitation Wavelength = 200 - 405, 200 - 488, 200 - 561, 200 - 642
 Filter Emission Wavelength = 419 - 470, 503 - 546, 576 - 617, 657 - 800
 Contrast Method = Fluorescence
 Illumination Wavelength = 561
 Channel Name = T2-Axiocam 820 #2-SR
 Excitation Wavelength = 561
 Emission Wavelength = 597
 Effective NA = 1.4
 Detection Wavelength = 419-470, 503-546, 576-617, 657-800
 Imaging Device = Axiocam 820 #2
 Camera Adapter = 1X
 Exposure Time = 100ms
 Depth of Focus = 0.92µm
 Binning Mode = 2,2
 Laser Wavelength = 561nm @1.00%
 Frame Time = 1.33s
 Scan Direction = Unidirectional
 Grating 32.0µm grating

DAPI -

Reflectors = SR HE LBF 405/488/561/642
 Beam Splitter = 405, 488, 561, 642
 Filter Excitation Wavelength = 200 - 405, 200 - 488, 200 - 561, 200 - 642
 Filter Emission Wavelength = 419 - 470, 503 - 546, 576 - 617, 657 - 800
 Contrast Method = Fluorescence
 Illumination Wavelength = 405
 Channel Name = T3-Axiocam 820 #2 -SR
 Excitation Wavelength = 405
 Emission Wavelength = 445
 Effective NA = 1.4
 Detection Wavelength = 419-470, 503-546, 576-617, 657-800
 Imaging Device = Axiocam 820 #2
 Camera Adapter = 1X
 Exposure Time = 50ms
 Depth of Focus = 0.69µm
 Binning Mode = 2,2
 Laser Wavelength = 640nm @10%
 Frame Time = 676.00ms
 Scan Direction = Unidirectional
 Grating 36.5µm grating

Post Processing - SIM2 Processing

Processing Dimension - 3D
 Result Sampling = 4
 Process Sampling = 4
 Channels = 3
 Algorithm = SIM2
 SIM Settings = Standard
 Auto Sharpness = On
 Sharpness = 8.8948 (690), 9.4656 (555), 7.8076 (DAPI)
 Order Combination = Weiner filter
 Regularization = None
 Regularization Weight = 0.0000
 Iterations = 3
 Filter = No Filter
 Fitting = Fast Fit
 Histogram = Scale to Min/Max

3D Image Processing

3D Maximum Projection = Precise
 Appearance = Threshold 1% (647), Threshold 1% (555), Threshold 1% (DAPI), Ramp 0% all channels, Maximum 100% all channels
 Background = Black
 Light = Brightness 125%, Enabled Tone Mapping
 Projection = View Angle 35°, Scale Z 275%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

Image Corrections

Identifyn® SRM Alexa Fluor™ 555 was pseudo-colored in Zen Software from yellow/orange, the default color, to white to provide visual contrast between the 555/680 channels.


DAPI was pseudo-colored in Zen Software from blue, the default color, to dark grey to provide visual contrast between the 555/680 and DAPI channels.

Image by P. Raut

Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE	
Catalog	SA-000070
Stage	SIM²
Instrument	ZEISS Elyra
Microscope configuration	Zeiss Elyra 5 Lattice SIM, AxioObserver.Z1/ 7 using Plan-Apochromat 63X/1.40 oil DIC M27, 1X Tubelens, was used with the following parameters for each dye:
Structured source metadata values	63
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	2469DA77EB8873BA4256533B9B771565E9F3DF0B3318475DD7C742C90054F4A4
Method PDF SHA-256	DEBFE98F9891274932CBE043269C65FEB29439828CC0608CC8227F490CD2404E

ORIGINAL IMAGE EVIDENCE / SINGLE-MOLECULE STORM

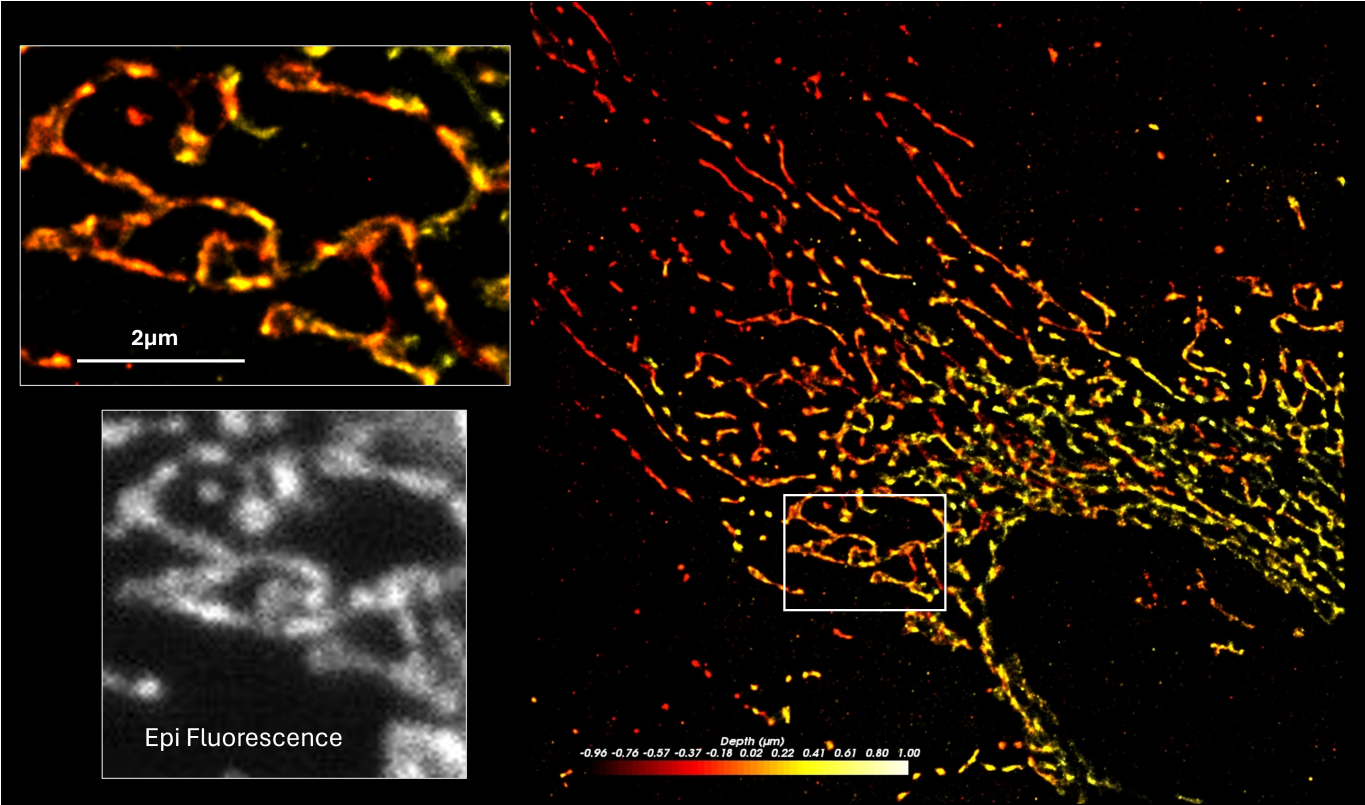

EVIDENCE TIER	Single-molecule STORM
INSTRUMENT	Bruker Vutara VXL
CELL MODEL	HeLa
DETECTED DYES	680
METADATA VALUES	71

STRUCTURED ACQUISITION METADATA / SINGLE-MOLECULE STORM

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Bruker Vutara VXL Biplane Single Molecule Microscope, using an Olympus 60X/1.30 silicon oil objective, was used with the following parameters:
Objective	Olympus 60X/1.30 silicon oil objective
Number of Probes	1
Number of Simultaneous Probes	1
Number of Reference Probes	1
Camera	Both Cameras
Color Channel	Both Channels
Probe Capture Mode	Interleaved
Z -Stack Capture Mode	Interleaved
Multiple Location Capture	Not selected
Post Record Reference	Not Selected
Fluidics	Not Selected
Autofocus Drift Correction	On
Biplane Module	635nm Dichroic
Objective	Silicon Selected
Stage Insert	Rectangular Selected
Course Focus Position	8-Well Chamber Selected
Dichroic	SuperRes
PSF	(Red, Orange)
Heater	Current: 26
Recording Vertical Field of View	100%
Widefield Camera Exposure Time	100ms 20ms
Super Resolution Camera Exposure Time	20ms
Widefield Camera Binning	1
Per-Probe Exposure Time	Selected
Predefined Probe	First probe: 640 nm (635 nm Dichroic); First reference probe: 640 nm (635 nm Dichroic)
Photoactivation/Imaging Laser	0% Selected
Exposure Time	20ms Selected
Record Workflow	Selected Options
View Mode	Widefield 200µm
Capture Mode	Live
Piezo Current	159 µm

FIELD	SOURCE-DOCUMENTED VALUE
Widefield 640nm	0.1X Neutral Density Filter: Selected, @1% Laser Input
Reference Probe 1 Laser control (640 nm (640 nm Dichroic))	Not Selected
Widefield camera Exposure Time	200ms
Widefield Laser	"Widefield 640nm" was deselected, and "calibrate" under Autofocus was selected.
Current Intensity	4.5
Calibration Value	-5070 nm/unit
Autofocus Mode	Pre-Capture
SuperRes	50µm is Selected
Piezo Record	Begin: 158.0; End: 158.0
SuperRes 640nm	0.1X Neutral Density Filter: Selected, @0.2% Laser Input
Record Workflow - Record Tab	Capture Parameters
Frames	Probe 1: 20000
Z Positions	1 using Steps: 0.2µm (200nm)
Cycles	1
Time Points	1
Pause Between Cycles	Not Selected
Automatic Photoactivation Laser Control	Not Selected
Laser Power	25%
Cutout Width	16 px
Max Frame Accumulation	1 frame
Max Accumulation Offset	1px
Fiducial at Max Accumulation	Not selected
Max Particles Per Frame	No Max
Background SLPE Removal	Not Selected
Cutout/Background Removal	Not Selected
Preview Cutout Positions	Selected
Probe1	BG threshold: 15
Sizing Mode	Radial
Particle size	4nm
Color by	Constant
Color Table	Single
Opacity Mode	Depth; Opacity 1: 0.03
Front-to-back Attenuation	Not Selected
Method	Particle (direct)
Time Intervals	7 Intervals

FIELD	SOURCE-DOCUMENTED VALUE
Pixel Size	50nm
Smoothing	8.00
PSF Z offset	-600 to +600
Radial precision	35
Axial precision	70

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 680 Affinity Purified Donkey Anti-Mouse, IgG (H + L)

Cat ID# - SA 000070

Hela cells were grown on μ -Slide 8 Well high Glass Bottom Ibidi chamber, followed by -20°C methanol fixation and blocked with Thermo Fisher Fish Serum Blocker cat#37527X3. The primary antibody, Mitochondria Antibody (MA5-12017), was incubated for 1 hour at room temperature at a dilution of 1:100. Cells were washed 3X in Identifyn's™ proprietary Wash Buffer and Identifyn® 680 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:100. Cells were washed 5X in Identifyn's™ proprietary Wash Buffer followed by the addition of Identifyn's™ proprietary STORM Buffer to the sample chamber enabling image acquisition.

Microscope

Bruker Vutara VXL Biplane Single Molecule Microscope, using an Olympus 60X/1.30 silicon oil objective, was used with the following parameters:

Calibration -

Calibration follows Identifyn's Calibration Standard Operating Procedure, which can be found here.

<https://identifyn.com/storm-calibration>

Image Acquisition -

SRX Software - Under the 'Single Molecule Localization' tab, 'Record' is selected and contains the following workflow tabs and parameters.

Configuration Tab - Capture Configuration

Number of Probes: 1

Number of Simultaneous Probes: 1

Number of Reference Probes: 1

Camera: Both Cameras

Color Channel: Both Channels

Probe Capture Mode: Interleaved

Z -Stack Capture Mode: Interleaved

Multiple Location Capture: Not selected

Post Record Reference: Not Selected

Fluidics: Not Selected

Autofocus Drift Correction: On

Microscope configuration

Biplane Module: 635nm Dichroic
 Objective: Silicon Selected
 Stage Insert: Rectangular Selected
 Course Focus Position: 8-Well Chamber Selected
 Dichroic: SuperRes
 PSF: (Red, Orange)
 Heater: Current: 26

Camera Configuration

Recording Vertical Field of View: 100%
 Widefield Camera Exposure Time: 100ms
 Super Resolution Camera Exposure Time: 20ms
 Widefield Camera Binning: 1
 Per-Probe Exposure Time: Selected

Probe Configuration

Predefined Probe: First probe: 640 nm (635 nm Dichroic); First reference probe: 640 nm (635 nm Dichroic)
 Photoactivation/Imaging Laser: 0% Selected
 Exposure Time: 20ms Selected

Experiment Configuration

Record Workflow: Selected Options
 View Mode: Widefield 200µm
 Capture Mode: Live

Stage and Piezo Selection

Examination of Sample

Cell(s) or Cellular Structure Localization - The red-bordered box identifies the area of the SuperRes view and defines a suitable cell(s) or cellular structure. The cell(s) or structures are optimally focused.

Piezo Current: 159 µm

Probe 1 Laser control (640 nm (635 nm Dichroic))

Widefield 640nm: 0.1X Neutral Density Filter: Selected, @1% Laser Input
 Reference Probe 1 Laser control (640 nm (640 nm Dichroic): Not Selected

Advanced Tools Option

Widefield camera Exposure Time: 200ms
 Default values are maintained unless otherwise noted.

Widefield Laser: "Widefield 640nm" was deselected, and "calibrate" under Autofocus was selected.

Autofocus - Calibration Values

Current Position" -0.979

Current Intensity: 4.5

Calibration Value: -5070 nm/unit

Autofocus Mode: Pre-Capture

View Mode

SuperRes: 50µm is Selected

Capture Mode

Live

Stage and Piezo Selection

Cell(s) or Cellular Structure Localization - Positioning of the target Cell or Subsection of the Target Cell is optimized and optimally focused.

Piezo Record: Begin: 158.0; End: 158.0

Probe 1 Laser control (640 nm (635 nm Dichroic)

SuperRes 640nm: 0.1X Neutral Density Filter: Selected, @0.2% Laser Input

Reference Probe 1 Laser control (640 nm (640 nm Dichroic)

Not Selected

Advanced Tools

Widefield Camera Exposure Time: 20ms

Default values are maintained unless otherwise noted.

Record Workflow - Record Tab: Capture Parameters

Frames: Probe 1: 20000

Z Positions:1 using Steps: 0.2µm (200nm)

Cycles: 1

Time Points: 1

Pause Between Cycles: Not Selected

Automatic Photoactivation Laser Control: Not Selected

Probe 1 Laser control (640 nm (635 nm Dichroic)

Laser Power: 25%

Expert Configuration Options - The Localization Tab

Beyond the values shown, all other parameters were default values.

Localization

Cutout Width: 16 px
 Max Frame Accumulation: 1 frame
 Max Accumulation Offset: 1px
 Fiducial at Max Accumulation: Not selected
 Max Particles Per Frame: No Max
 Background SLPE Removal: Not Selected
 Cutout/Background Removal: Not Selected
 Preview Cutout Positions: Selected

Record Workflow - Localization Tab

Data Collection

The folder is created automatically with the localization file for this image acquisition.

Recording Summary

All parameters were carried over from previous tabs and are kept except:

Probe1: BG threshold: 15

Region of Interest -

Not selected

Display

Was deployed to inspect if the BG threshold applied chooses localizations in an expected manner

Record Workflow - View Tab

Region of Interest

Default values

Visualization Parameters

Point Splatting
 Sizing Mode: Radial
 Particle size: 4nm
 Color by: Constant
 Color Table: Single
 Opacity Mode: Depth; Opacity 1: 0.03
 Front-to-back Attenuation: Not Selected

Post Acquisition analysis - View Tab

Drift Correction - Computed with the following parameters:

Method: Particle (direct)
 Time Intervals: 7 Intervals
 Pixel Size: 50nm
 Smoothing: 8.00

Advanced Particle Filters - Applied to the drift-corrected data with the following parameters

PSF Z offset: -600 to +600

Radial precision: 35

Axial precision: 70

The other parameters were not applied.

Statistical analysis - NA


Image by S. Thakur

Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE

Catalog	SA-000070
Stage	Single-molecule STORM
Instrument	Bruker Vutara VXL
Microscope configuration	Bruker Vutara VXL Biplane Single Molecule Microscope, using an Olympus 60X/1.30 silicon oil objective, was used with the following parameters:
Structured source metadata values	71
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	CCF66615A113E5D0249DC0C5A97769BF3E84664E02A68E5975DA4FC9DA06B2A2
Method PDF SHA-256	8FDE97E908338685022B2D2C299F9ACB16203868504BDD3565FF34B45AE046F9

ORIGINAL IMAGE EVIDENCE / CONTROL

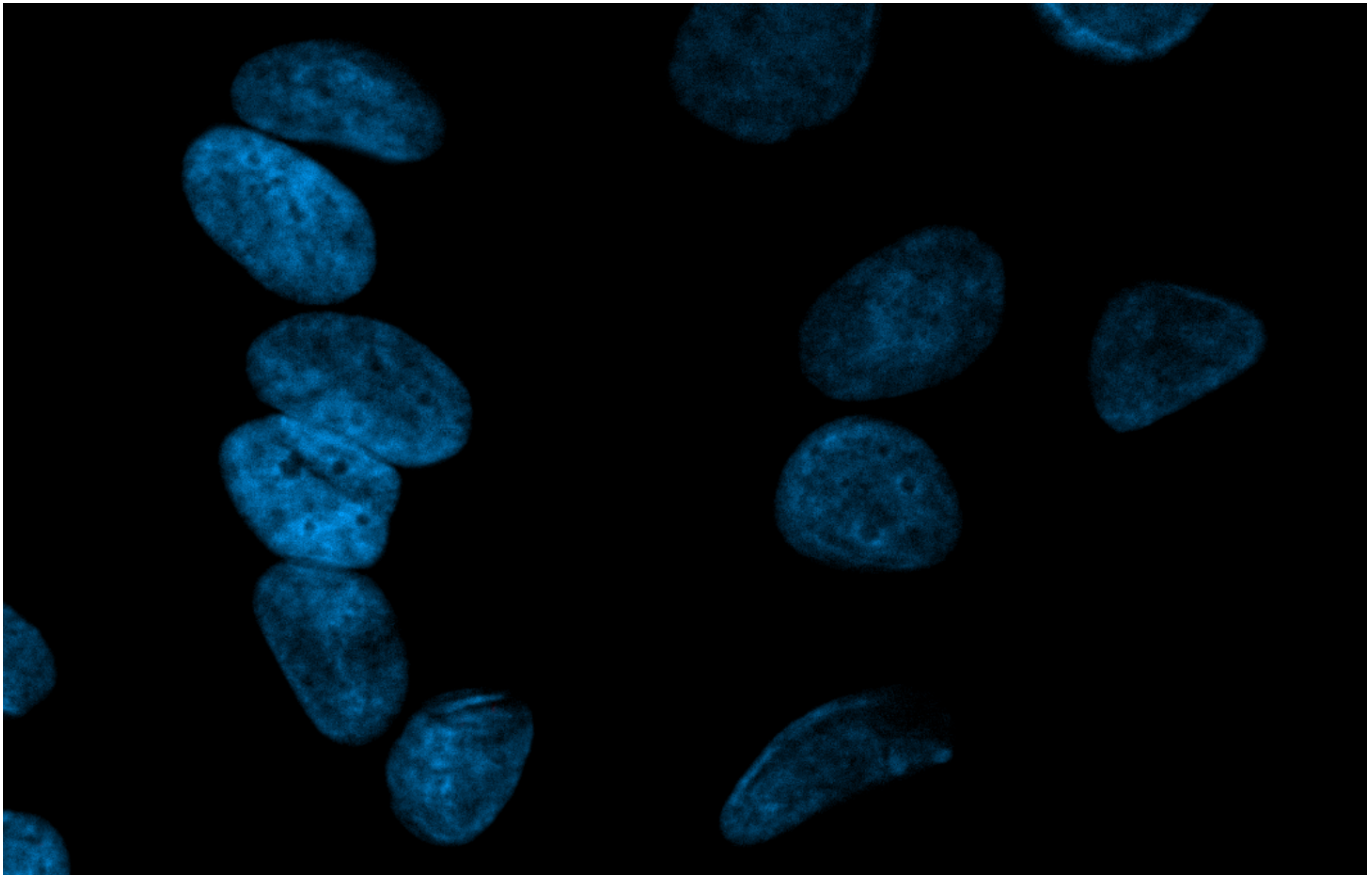

EVIDENCE TIER	Control
INSTRUMENT	ZEISS Axio Observer.Z1/7 Apotome
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 680
METADATA VALUES	32

STRUCTURED ACQUISITION METADATA / CONTROL

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:
Objective	EC Plan-Neofluar 63X/1.25 oil M27
Channels	2
Scaling (Per Pixel)	0.143µm X 0.143µm
Image Size (Pixels)	1067 X 686
Image Size (Scaled)	152.43µm X 98.00µm
Bit Depth	14 Bit
Image Center Position	X: 74.97mm, Y: 47.68mm
Stage Position	X: 74.97mm, Y: 47.68mm
ROI Center Offset	X: 1.14µm, Y: 0.00µm
Reflector	50 Cy5 49 DAPI
Beam Splitter	660 395
Filter Excitation Wavelength	625 - 655 335-383
Filter Emission Wavelength	665 - 715 420-470
Contrast Method	Fluorescence
Light source	X-Cite Xylis Lamp Intensity @25% X-Cite Xylis Lamp Intensity @10%
Exposure Time	300ms 30ms
Excitation Wavelength	679 353
Emission Wavelength	702 465
Effective NA	1.25
Imaging Device	Axiocam 807
Camera Adapter	1X
Depth of Focus	1.36µm 0.90µm
Binning Mode	2,2
Apotome SIM Image Processing	Display Mode "Optical Sectioning" - enabled correction selected.

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 680 Affinity Purified Donkey Anti-Mouse IgG (H + L)

Cat ID# - SA 000070

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher Fish Serum Blocker cat#37527X3. In the absence of a primary antibody, the Identifyn® 680 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:

Single Plane (2D)

Channels = 2

Scaling (Per Pixel) = 0.143µm X 0.143µm

Image Size (Pixels) = 1067 X 686

Image Size (Scaled) = 152.43µm X 98.00µm

Bit Depth = 14 Bit

Image Center Position = X: 74.97mm, Y: 47.68mm

Stage Position = X: 74.97mm, Y: 47.68mm

ROI Center Offset = X: 1.14µm, Y: 0.00µm

680 -

Reflector = 50 Cy5

Beam Splitter = 660

Filter Excitation Wavelength = 625 - 655

Filter Emission Wavelength = 665 - 715

Contrast Method = Fluorescence

Light source = X-Cite Xylis Lamp Intensity @25%

Exposure Time = 300ms

Excitation Wavelength = 679

Emission Wavelength = 702

Effective NA = 1.25

Imaging Device = Axiocam 807

Camera Adapter = 1X

Depth of Focus = 1.36µm

Binning Mode = 2,2

DAPI -

Reflector = 49 DAPI
 Beam Splitter = 395
 Filter Excitation Wavelength = 335-383
 Filter Emission Wavelength = 420-470
 Contrast Method = Fluorescence
 Light source = X-Cite Xylis Lamp Intensity @10%
 Exposure Time = 30ms
 Excitation Wavelength = 353
 Emission Wavelength = 465
 Effective NA = 1.25
 Imaging Device = Axiocam 807
 Camera Adapter = 1X
 Depth of Focus = 0.90µm
 Binning Mode = 2,2

Post Processing - SIM Processing

Apotome SIM Image Processing = Display Mode "Optical Sectioning" - enabled correction selected.

Normalization, Phase Corrector, Fourier Filter, and Deconvolution were NOT used.

Image Corrections

None

Control Summary -

In the absence of a primary antibody, Identifyn Standards for Optical Microscopy Methods™ were applied using standard staining methodology and image acquisition settings using the Zeiss Apotome SIM. With no image correction, the image demonstrates that the secondary antibody, minus a primary target, had no off-target binding and no significant presence of free dye within the sample.

The control data suggests the secondary antibody is highly specific and free of unconjugated (free) dye post-conjugation.

Image by J.K. Bennett

Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE

Catalog	SA-000070
Stage	Control
Instrument	ZEISS Axio Observer.Z1/7 Apotome
Microscope configuration	Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:
Structured source metadata values	32

SOURCE PROVENANCE

Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	B70D283E48AAD16439B2F1B13A928A9E0E738F904A2E67C1C009AF5C011F64C1
Method PDF SHA-256	2E1F50ABDAFDFA29C23E009B262127BD264CAA59F07438654FD0E25CB32BDD7C