

IDENTIFYN RESOLUTION STEPDOWN

SECONDARY ANTIBODY MICROSCOPY EVIDENCE ASSESSMENT

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit, IgG (H + L)

WESTERN BLOT -> WIDEFIELD -> WIDEFIELD SIM / APOTOME -> CONFOCAL -> AIRYSCAN
SIM -> SIM² -> SINGLE-MOLECULE STORM

8


ORDERED EVIDENCE TIERS

1

SUPPORTING CONTROL

PENDING

SCIENTIST REVIEW

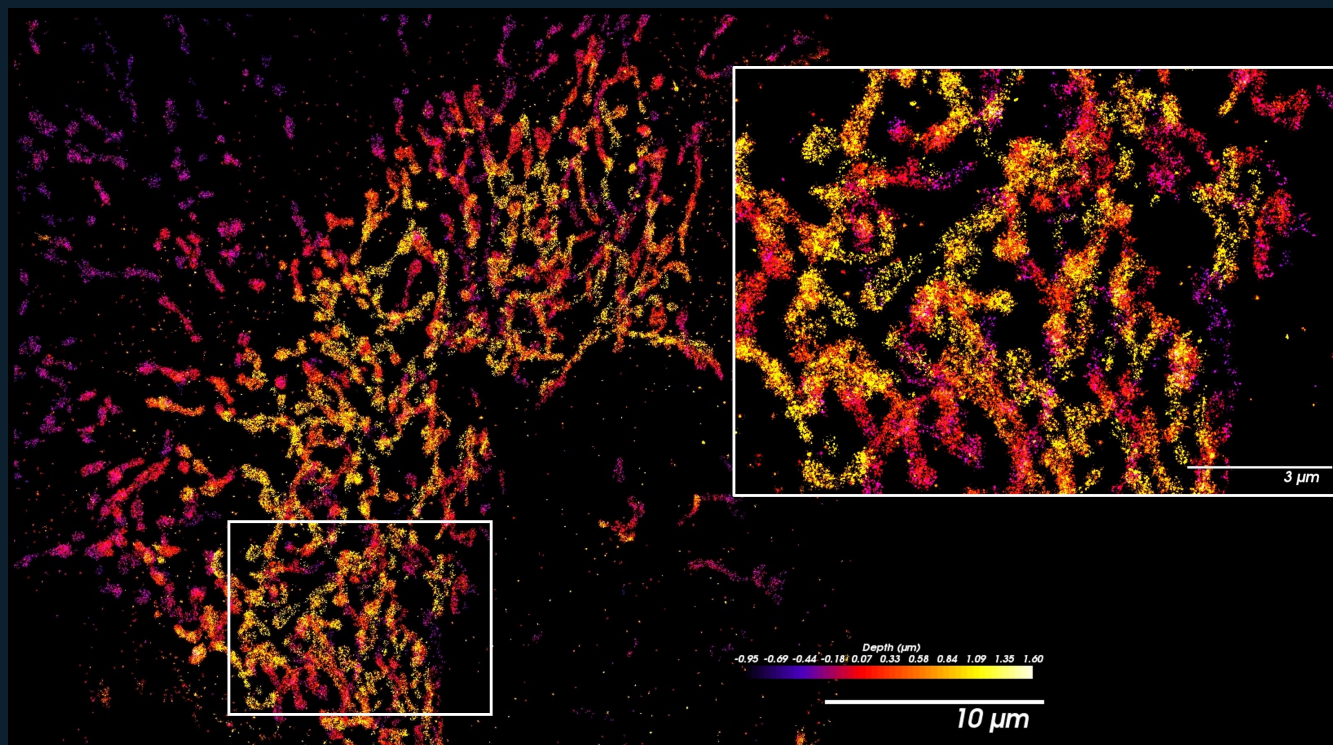

REPRESENTATIVE HIGHEST-AVAILABLE VIEW / SINGLE-MOLECULE STORM

SA-000035 | PRODUCT-LEVEL EVIDENCE DOSSIER

SOURCE-GROUNDED MICROSCOPY + BIOLOGICAL REVIEW / IDENTIFYN EVIDENCE PRESERVED

CRO CAPABILITY DEMONSTRATED

Identifyn performed the experimental and imaging work documented below. BENNETT converts that operating history into a governed, source-bounded scientific record.

- Source-documented sample preparation and antibody/reagent workflow
- Western blot imaging
- Widefield fluorescence microscopy
- Widefield structured illumination / Apotome optical sectioning
- Confocal microscopy
- Airyscan acquisition and reconstruction workflow
- Structured illumination microscopy
- SIM² reconstruction workflow
- Single-molecule STORM presentation workflow
- Preserved control experiment
- Z-stack / 3D acquisition
- Multi-channel imaging

SCIENTIFIC QUESTION

What source-bounded experimental and microscopy evidence is preserved for Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit, IgG (H + L), and what is the strongest interpretation allowed by the available modalities and controls?

EVIDENCE AVAILABLE

Western blot -> Widefield -> Widefield SIM — Apotome -> Confocal -> Airyscan -> SIM -> SIM² -> Single-molecule STORM
-> Control

BENNETT ASSESSMENT

The preserved SA-000035 record contains the full ordered evidence sequence from Western blot through single-molecule STORM. Each modality retains its own acquisition and processing boundary.

BENNETT / MICROSCOPY AND BIOLOGICAL EVIDENCE REVIEW

SOURCE-GROUNDED RETROSPECTIVE REVIEW / PENDING SCIENTIST REVIEW

SOURCE STATE	SOURCE HASH VERIFIED / EVENT RECORDED
BENNETT EVIDENCE REVIEW	COMPLETED / SOURCE-BOUNDED
NATIVE IMAGE REPROCESSING	NOT PERFORMED
LITERATURE SOURCES	INDEPENDENTLY VERIFIED
SCIENTIST REVIEW	PENDING
PUBLICATION	NOT AUTHORIZED

OVERALL CALL / FULL STEPDOWN / SOURCE-BOUNDED REVIEW

The preserved SA-000035 record contains the full ordered evidence sequence from Western blot through single-molecule STORM. Each modality retains its own acquisition and processing boundary.

SETTINGS ASSESSMENT

The record preserves 8 ordered evidence tier(s). Structured source metadata values are reported by stage and remain tied to the original method objects.

BIOLOGICAL SUPPORT

The record supports retrospective, source-bounded microscopy review. Target identity, specificity, treatment effect, binding, interaction and mechanism are not inferred from presentation images alone.

CONTROL ASSESSMENT

A true preserved control record is present and appears last.

CLAIM CEILING

This draft supports historical capability documentation, source registration, modality ordering, settings review and bounded interpretation. It does not independently validate antibody specificity, quantify a population response, establish binding, interaction, causation or mechanism, or authorize publication.

PROCESSING DISCLOSURE

Retrospective BENNETT architectural evaluation of preserved Identifyn source evidence. BENNETT did not perform native-file reprocessing, new deterministic measurement or the historical image post-processing represented in this record.

REAGENTS AND ACQUIRED CHANNELS

Preparation reagents are reported separately from channels actually documented in the acquisition settings. Fluorophores mentioned in staining are not automatically treated as acquired channels.

EVIDENCE OBJECT	REAGENTS / FLUOROPHORES PRESENT	CHANNELS ACTUALLY ACQUIRED
Western blot	555	Not deterministically stated in the acquisition block
Widefield	405/DAPI; 555	2; 45 Texas Red; 49 DAPI; 540 - 580; 335 - 383; 593 - 668; 420 - 470; 553
Widefield SIM — Apotome	405/DAPI; 555	2; 45 Texas Red; 49 DAPI; 540 - 580; 335-383; 593 - 668; 420-470; 553
Confocal	405/DAPI; 488; 555	2; None; 561nm @1.0%; 405nm @0.7%; 553; 353; 568; 465
Airyscan	405/DAPI; 488; 555	2; None; 561nm @0.5%; 405nm @0.5%; 553; 353; 568; 465
SIM	405/DAPI; 488; 555	2; 1; SR HE LBF 405/488/561/642; 200 - 405, 200 - 488, 200 - 561, 200 - 642; 419 - 470, 503 - 546, 576 - 617, 657 - 800; T2-Axiocam 820 #2-SR; 561; 405
SIM ²	405/DAPI; 488; 555	2; 642nm @10.0%; 405nm @10.0%; 642; 405; 655; 515; 561.000000
Single-molecule STORM	555	Both Channels
Control	405/DAPI; 555	2; AF532-49014; 49 DAPI; 515 - 545; 335 - 383; 555 - 595; 420 - 470; 553

MODALITY ASSESSMENT / PART 1 OF 9

Western blot / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: Azure Sapphire FL. Objective: not explicitly stated. Platform: Azure Sapphire FL with Customizable Laser and Filter Modules, Enabling UV- NIR and Z-Plane(s). Structured source metadata values: 11.

VISIBLE OBSERVATION

A preserved presentation image is available for Western blot. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Western blot, documents platform context as Azure Sapphire FL, and records detected dye/channel descriptors as 555.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy and antibody-validation guidance that presentation evidence must remain bounded by modality, controls and source documentation.

INTERPRETIVE LIMIT

Band position and displayed intensity do not independently establish analytical specificity, target identity, linearity, or treatment effect.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Western blot evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 2 OF 9

Widefield / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS Axio Imager.M1. Objective: Plan-Apochromat 63x/1.40 Oil M27. Platform: Zeiss Axio Imager.M1 Widefield, using a Plan-Apochromat 63x/1.40 Oil M27, Axiocam MR R3, and X-Cite Xylis Lamp was used with the following parameters for each dye: Acquisition: Channels: 2; Scaling (Per Pixel): 0.102µm X 0.102µm; Image size (Pixels): 607 X 486; Image Size (Pixels): 607 X 486; Bit Depth: 12 Bit. Detector/camera: Imaging Device: Axiocam MR R3. Timing: Exposure Time: 100ms; 80ms. Illumination: Light source: X-Cite Xylis Lamp Intensity @29%; X-Cite Xylis Lamp Intensity @15%. Optical/scan: Effective NA: 1.4. Structured source metadata values: 30.

VISIBLE OBSERVATION

A preserved presentation image is available for Widefield. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Widefield, documents platform context as ZEISS Axio Imager.M1, and records detected dye/channel descriptors as 405/DAPI; 555.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy and antibody-validation guidance that presentation evidence must remain bounded by modality, controls and source documentation.

INTERPRETIVE LIMIT

A presentation image supports gross localization and source-bounded co-occurrence, not direct binding, molecular colocalization, or native quantitative measurement.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Widefield evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 3 OF 9

Widefield SIM — Apotome / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS Axio Observer.Z1/7 Apotome. Objective: EC Plan-Neofluar 63X/1.25 oil M27. Platform: Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, AxioCam 807, and X-Cite Xylys Lamp was used with the following parameters for each dye: Acquisition: Channels: 2; Scaling (Per Pixel): 0.143µm X 0.143µm; Image size (Pixels): 931 X 837; Image Size (Pixels): 931 X 837; Bit Depth: 14 Bit. Detector/camera: Imaging Device: AxioCam 807. Timing: Exposure Time: 120ms; 40ms. Illumination: Light source: X-Cite Xylys Lamp Intensity @37%; X-Cite Xylys Lamp Intensity @5%. Optical/scan: Effective NA: 1.25. Structured source metadata values: 32.

VISIBLE OBSERVATION

A preserved presentation image is available for Widefield SIM — Apotome. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Widefield SIM — Apotome, documents platform context as ZEISS Axio Observer.Z1/7 Apotome, and records detected dye/channel descriptors as 405/DAPI; 555.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy and antibody-validation guidance that presentation evidence must remain bounded by modality, controls and source documentation.

INTERPRETIVE LIMIT

Improved optical sectioning does not by itself establish reconstructed super-resolution or molecular interaction.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Widefield SIM — Apotome evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 4 OF 9

Confocal / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS LSM 900. Objective: with a Plan-Apochromat 63X/1.40 oil DIC M27. Platform: Zeiss LSM 900 Confocal, Axio Observer.Z1/7, using with a Plan-Apochromat 63X/1.40 oil DIC M27 was used with the following parameters for each dye:. Acquisition: Channels: 2; Scaling (Per Pixel): 0.071µm X 0.071µm; Image size (Pixels): 523 X 509; Image Size (Pixels): 523 X 509; Bit Depth: 16 Bit. Detector/camera: Imaging Device: Airyscan; Detector Type: GaAsP-PMT. Timing: Pixel Time: 0.51µs; Frame Time: 10.15s. Illumination: Laser Wavelength: 561nm @1.0%; 405nm @0.7%. Optical/scan: Pinhole: 1.00AU / 49µm; 1.00AU / 37µm; Scan Zoom: 1.4; LSM Scan Speed: 9; Scan Direction: Bidirectional; Effective NA: 1.4. Structured source metadata values: 38.

VISIBLE OBSERVATION

A preserved presentation image is available for Confocal. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Confocal, documents platform context as ZEISS LSM 900, and records detected dye/channel descriptors as 405/DAPI; 488; 555.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy and antibody-validation guidance that presentation evidence must remain bounded by modality, controls and source documentation.

INTERPRETIVE LIMIT

Optical sectioning and source-bounded 3D presentation do not establish binding, mechanism, or population-level effect.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Confocal evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 5 OF 9

Airyscan / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS LSM 900. Objective: with a Plan-Apochromat 63X/1.40 oil DIC M27. Platform: Zeiss LSM 900 Confocal, Axio Observer.Z1/7, using with a Plan-Apochromat 63X/1.40 oil DIC M27 was used with the following parameters for each dye:. Acquisition: Z-Stack: 65 Slices (3.20µm); Channels: 2; Scaling (Per Pixel): 35.29nm X 35.29nm X 50.00nm; Image size (Pixels): 1141 X 1165; Image Size (Pixels): 1141 X 1165; Bit Depth: 16 Bit. Detector/camera: Imaging Device: Airyscan; Detector Type: GaAsP-PMT. Timing: Pixel Time: 0.55µs; Frame Time: 9.48s. Illumination: Laser Wavelength: 561nm @0.5%; 405nm @0.5%. Optical/scan: Pinhole: 5.00AU / 245µm; 5.00AU / 188µm; Scan Zoom: 1.5; LSM Scan Speed: 7; Scan Direction: Bidirectional; Effective NA: 1.4. Processing: Projection: View Angle 35°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected); Background: Black; AiryScan Mode: Super Resolution 10.0 (3D, Auto); Super Resolution 8.8 (3D, Auto). Structured source metadata values: 50.

VISIBLE OBSERVATION

A preserved presentation image is available for Airyscan. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Airyscan, documents platform context as ZEISS LSM 900, and records detected dye/channel descriptors as 405/DAPI; 488; 555.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy guidance that advanced-resolution outputs remain dependent on acquisition, reconstruction or localization quality control.

INTERPRETIVE LIMIT

Displayed feature separation remains reconstruction dependent; no unsupported numerical resolution or molecular architecture claim is permitted.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Airyscan evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 6 OF 9

SIM / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS Elyra. Objective: Plan-Apochromat 63X/1.40 oil DIC M27. Platform: Zeiss Elyra 5 Lattice SIM, AxioObserver.Z1/ 7 using Plan-Apochromat 63X/1.40 oil DIC M27, 1X Tubelens, was used with the following parameters for each dye:. Acquisition: Z-Stack: 39 Slices (1.9µm); Channels: 2; 1; Scaling (Per Pixel): 42.23nm X 42.23nm X 50.00nm; Image size (Pixels): 2528 X 2528; Image Size (Pixels): 2528 X 2528; Bit Depth: 16 Bit. Detector/camera: Imaging Device: AxioCam 820#2. Timing: Exposure Time: 75ms; 50ms; Frame Time: 1.33s; 676.00ms. Illumination: Laser Wavelength: 561nm @0.5%; 405nm @1.0%; Illumination Wavelength: 561; 405. Optical/scan: Scan Direction: Unidirectional; Effective NA: 1.4. Processing: Algorithm: SIM; Process Sampling: 2; Result Sampling: 2; Projection: View Angle 61°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected); Background: Black. Structured source metadata values: 54.

VISIBLE OBSERVATION

A preserved presentation image is available for SIM. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as SIM, documents platform context as ZEISS Elyra, and records detected dye/channel descriptors as 405/DAPI; 488; 555.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy guidance that advanced-resolution outputs remain dependent on acquisition, reconstruction or localization quality control.

INTERPRETIVE LIMIT

Reconstruction-dependent structural separation requires native reconstruction QC before numerical resolution or molecular dimensions can be claimed.

CLAIM CEILING

This tier supports a source-bounded statement that the historical SIM evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 7 OF 9

SIM² / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS Elyra 7. Objective: Plan-Apochromat 63X/1.46 oil Korr M27. Platform: Zeiss Elyra 7, Andor1, AxioObserver, using Plan-Apochromat 63X/1.46 oil Korr M27 was used with the following parameters for each dye: Acquisition: Z-Stack: 6 Slices (350nm); Channels: 2; Scaling (Per Pixel): 15.65nm X 15.65nm X 70.00nm; Image size (Pixels): 1683 X 1965; Image Size (Pixels): 1683 X 1965; Bit Depth: 16 Bit. Detector/camera: Imaging Device: Edge 4.2 SIM; Detector Type: Camera. Timing: Exposure Time: 120ms; 100ms; Frame Time: 1.0s. Illumination: Laser Wavelength: 642nm @10.0%; 405nm @10.0%. Optical/scan: Scan Zoom: 1.0; Scan Direction: Unidirectional; Averaging: 16; Effective NA: 1.46. Processing: Projection: View Angle 35°, Scale Z 51%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected); Background: Black. Structured source metadata values: 62.

VISIBLE OBSERVATION

A preserved presentation image is available for SIM². BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as SIM², documents platform context as ZEISS Elyra 7, and records detected dye/channel descriptors as 405/DAPI; 488; 555.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy guidance that advanced-resolution outputs remain dependent on acquisition, reconstruction or localization quality control.

INTERPRETIVE LIMIT

Further reconstruction-dependent segmentation does not establish molecular dimensions, structure identity, or mechanism without independent support.

CLAIM CEILING

This tier supports a source-bounded statement that the historical SIM² evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 8 OF 9

Single-molecule STORM / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: Bruker Vutara VXL. Objective: Olympus 60X/1.30 silicon oil objective. Platform: Bruker Vutara VXL Biplane Single Molecule Microscope, using an Olympus 60X/1.30 silicon oil objective, was used with the following parameters:.

Detector/camera: Camera: Both Cameras. Timing: Exposure Time: 20ms Selected; Super Resolution Camera Exposure Time: 20ms; Widefield Camera Exposure Time: 100ms. Illumination: Photoactivation/Imaging Laser: 0% Selected.

Structured source metadata values: 79.

VISIBLE OBSERVATION

A preserved presentation image is available for Single-molecule STORM. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Single-molecule STORM, documents platform context as Bruker Vutara VXL, and records detected dye/channel descriptors as 555.

LITERATURE CORRELATION

Consistent with peer-reviewed microscopy guidance that advanced-resolution outputs remain dependent on acquisition, reconstruction or localization quality control.

INTERPRETIVE LIMIT

Without localization tables, uncertainty, blinking, drift, and independent cluster evidence, the presentation cannot establish molecule count, cluster truth, exact precision, or molecular architecture.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Single-molecule STORM evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

MODALITY ASSESSMENT / PART 9 OF 9

Control / SOURCE EVIDENCE PRESERVED

DOCUMENTED SETTINGS

Platform: ZEISS Axio Observer.Z1/7 Apotome. Objective: EC Plan-Neofluar 63X/1.25 oil M27. Platform: Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:. Acquisition: Channels: 2; Scaling (Per Pixel): 0.143µm X 0.143µm; Image size (Pixels): 1279 X 1100; Image Size (Pixels): 1279 X 1100; Bit Depth: 14 Bit. Detector/camera: Imaging Device: Axiocam 807 mono. Timing: Exposure Time: 200ms; 30ms. Illumination: Light source: X-Cite Xylis Lamp Intensity @25%; X-Cite Xylis Lamp Intensity @10%. Optical/scan: Effective NA: 1.25. Structured source metadata values: 32.

VISIBLE OBSERVATION

A preserved presentation image is available for Control. BENNETT records the visible source presentation without creating a new native measurement.

SOURCE-REPORTED RESULT

The source identifies this object as Control, documents platform context as ZEISS Axio Observer.Z1/7 Apotome, and records detected dye/channel descriptors as 405/DAPI; 555.

LITERATURE CORRELATION

Consistent with peer-reviewed antibody-control guidance that a no-primary or related control bounds background but is not a complete specificity system.

INTERPRETIVE LIMIT

A control bounds the recorded comparison only; it does not establish universal specificity, zero background, zero cross-reactivity, or absence of free dye.

CLAIM CEILING

This tier supports a source-bounded statement that the historical Control evidence and documented settings are preserved for review; stronger biological or quantitative conclusions require compatible native data, controls and scientist review.

CROSS-MODALITY SYNTHESIS

The preserved SA-000035 record contains the full ordered evidence sequence from Western blot through single-molecule STORM. Each modality retains its own acquisition and processing boundary.

Different acquisitions are not treated as a quantitative intensity ladder. Any continuity statement remains qualitative and source bounded.

BENNETT LITERATURE CORRELATION — SOURCES INDEPENDENTLY VERIFIED

BENNETT uses independently verified primary scientific sources to test whether the interpretation is scientifically consistent and properly bounded. Literature correlation does not retroactively validate the Identifyn dataset or replace scientist review.

- Antibody and microscopy evidence require orthogonal controls and modality-appropriate interpretation; presentation images alone do not establish analytical specificity.
- Advanced-resolution presentation depends on acquisition, reconstruction or localization quality control before numerical resolution, molecular dimensions or cluster identity can be claimed.

REFERENCES

1. Uhlen M, et al. A proposal for validation of antibodies. Nat Methods. 2016;13:823-827. doi:10.1038/nmeth.3995.
2. Gustafsson MGL. Surpassing the lateral resolution limit by a factor of two using structured illumination microscopy. J Microsc. 2000;198:82-87. doi:10.1046/j.1365-2818.2000.00710.x.
3. Sage D, et al. Quantitative evaluation of software packages for single-molecule localization microscopy. Nat Methods. 2015;12:717-724. doi:10.1038/nmeth.3442.

RELEASE BOUNDARY

This assessment remains a draft pending scientist review. No publication is authorized. Any future native-file analysis must enter BENNETT as a new evidence snapshot with routed engine authority, native-data QA, methods, limitations, and an independently reviewed claim ceiling.

SOURCE RECONCILIATION / QA / PROVENANCE

SOURCE STATUS - PRESERVED / AUTO-RECONCILED

Historical Identifyn source material was subjected to BENNETT retrospective QA. Original source state and correction history remain preserved in provenance.

HIGH CONFIDENCE - AUTO-RECONCILED

Airyscan / Scaling (Per Pixel): 35.29nm X 35.29nm X 50.00nm -> 0.03529 μ m X 0.03529 μ m X 0.05000 μ m. Both numerical magnitude and unit were normalized, then checked against the reported field dimensions; no unit label was changed alone. Supporting evidence: Image Size (Pixels)=1141 X 1165; Image Size (Scaled)=40.26 μ m X 41.11 μ m; PASS - INTERNALLY CONSISTENT. Documented sampling reproduces the reported physical field dimensions. Maximum field-dimension error 0.01%.

HIGH CONFIDENCE - AUTO-RECONCILED

SIM / Scaling (Per Pixel): 42.23nm X 42.23nm X 50.00nm -> 0.04223 μ m X 0.04223 μ m X 0.05000 μ m. Both numerical magnitude and unit were normalized, then checked against the reported field dimensions; no unit label was changed alone. Supporting evidence: Image Size (Pixels)=2528 X 2528; Image Size (Scaled)=106.75 μ m X 106.75 μ m; PASS - INTERNALLY CONSISTENT. Documented sampling reproduces the reported physical field dimensions. Maximum field-dimension error 0.01%.

HIGH CONFIDENCE - AUTO-RECONCILED

SIM² / Scaling (Per Pixel): 15.65nm X 15.65nm X 70.00nm -> 0.01565 μ m X 0.01565 μ m X 58.33333 μ m. Both numerical magnitude and unit were normalized, then checked against the reported field dimensions; no unit label was changed alone. Supporting evidence: Image Size (Pixels)=1683 X 1965; Image Size (Scaled)=26.34 μ m X 30.76 μ m; PASS - INTERNALLY CONSISTENT. Documented sampling reproduces the reported physical field dimensions. Maximum field-dimension error 0.03%.

BENNETT EVIDENCE REVIEW COMPLETE

INTERPRETATION TO EVIDENCE

BENNETT has completed the bounded retrospective assessment.
The following pages switch ownership to the preserved Identifyn record.



IDENTIFYN PRESERVED SOURCE EVIDENCE

ORIGINAL RECORD BEGINS

Images, source methods, acquisition settings and provenance follow in the locked
Stepdown order. Scientific wording is preserved; missing modalities are not invented.
A preserved control follows all available Stepdown tiers as supporting evidence.

PRODUCT-LEVEL STEPDOWN MAP


This dossier preserves the complete available evidence progression for SA-000035. Each tier remains tied to its original image, source method, instrument context and cryptographic identity. A preserved control is retained as supporting evidence and appears after every resolution tier.

CANONICAL STEPDOWN	EVIDENCE STAGE	INSTRUMENT	STATUS
1	Western blot	Azure Sapphire FL	PRESERVED
2	Widefield	ZEISS Axio Imager.M1	PRESERVED
3	Widefield SIM - Apotome	ZEISS Axio Observer.Z1/7 Apotome	PRESERVED
4	Confocal	ZEISS LSM 900	PRESERVED
5	Airyscan	ZEISS LSM 900	PRESERVED
6	SIM	ZEISS Elyra	PRESERVED
7	SIM ²	ZEISS Elyra 7	PRESERVED
8	Single-molecule STORM	Bruker Vutara VXL	PRESERVED

INTERPRETIVE BOUNDARY

Ordering evidence by resolution tier does not make the modalities interchangeable. Each stage retains its acquisition environment and scientific limitations. This pilot organizes the record; it does not synthesize new biological claims.

ORIGINAL IMAGE EVIDENCE / WESTERN BLOT

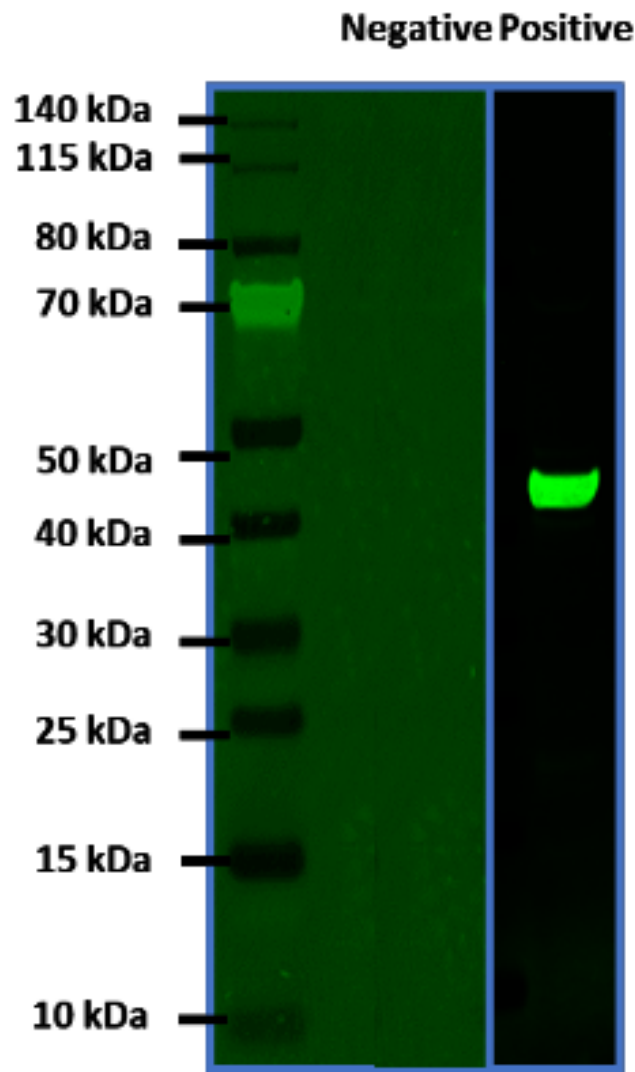

EVIDENCE TIER	Western blot
INSTRUMENT	Azure Sapphire FL
CELL MODEL	HeLa
DETECTED DYES	555
METADATA VALUES	11

STRUCTURED ACQUISITION METADATA / WESTERN BLOT

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Azure Sapphire FL with Customizable Laser and Filter Modules, Enabling UV- NIR and Z-Plane(s)
Scanner	Azure Sapphire FL with Customizable Laser and Filter Modules, Enabling UV- NIR and Z-Plane(s)
Detection mode	Fluorescence
Laser	532nm
Emission Filter	572±28nm
Detector	Avalanche Photodiode
Intensity	L1
Pixel size	100 µm
Scan Speed	High
Quality	High
Focus	Membrane (0 µm in Z-axis)
Image	Identifyn® LLC

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit IgG (H + L)

Cat ID# - SA 000035

HeLa cells were homogenized using an ultrasonication probe and centrifuged to pellet down the cell debris. The supernatant of the lysate was mixed with NuPAGE™ LDS Sample Buffer (4X), heated at 80oC for 10 min, and subjected to electrophoresis using NuPAGE™ 4 to 12%, Bis-Tris, 1.0-1.5 mm, Mini Protein Gels in a Mini Gel Tank. The Thermo Fisher's PageRuler™ Prestained Protein Ladder, 10 to 180 kDa, was used as a molecular weight marker.

Post electrophoresis, the proteins were transferred to a polyvinylidene difluoride (PVDF) membrane using iBlot™ 3 Starter Kit, PVDF. The transfer membrane was blocked with Blocker™ Casein for 1 hour and washed 5X with PBS. The blocked membrane was incubated with Actin Recombinant Monoclonal Antibody (JF47-01) (MA5-32530) for 2 hours, followed by 5X PBS washes. Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat anti-Rabbit IgG was incubated for 1 hour, followed by washing 5X with PBS. The membrane was dried for 10 minutes at room temperature before imaging.

Scanner = Azure Sapphire FL with Customizable Laser and Filter Modules, Enabling UV- NIR and Z-Plane(s)

Scan Settings

Detection mode = Fluorescence

Laser = 532nm

Emission Filter = 572±28nm

Detector = Avalanche Photodiode

Intensity = L1

Pixel size = 100 µm

Scan Speed = High

Quality = High

Focus = Membrane (0 µm in Z-axis)

Post Processing

None

Image: Identifyn® LLC

Copyright 2026 GMD12 LLC.


SOURCE PROVENANCE

Catalog	SA-000035
Stage	Western blot
Instrument	Azure Sapphire FL

SOURCE PROVENANCE

Microscope configuration	Azure Sapphire FL with Customizable Laser and Filter Modules, Enabling UV- NIR and Z-Plane(s)
Structured source metadata values	11
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	4D1D2B6B1D2DCF6D1FE177B10CE191C9C6A951B65E525240E63FE6675BF5F3B5
Method PDF SHA-256	72D002813755EA0D64DEFB17302B56B695F3C152D2468C4BF23E810F242EA786

ORIGINAL IMAGE EVIDENCE / WIDEFIELD

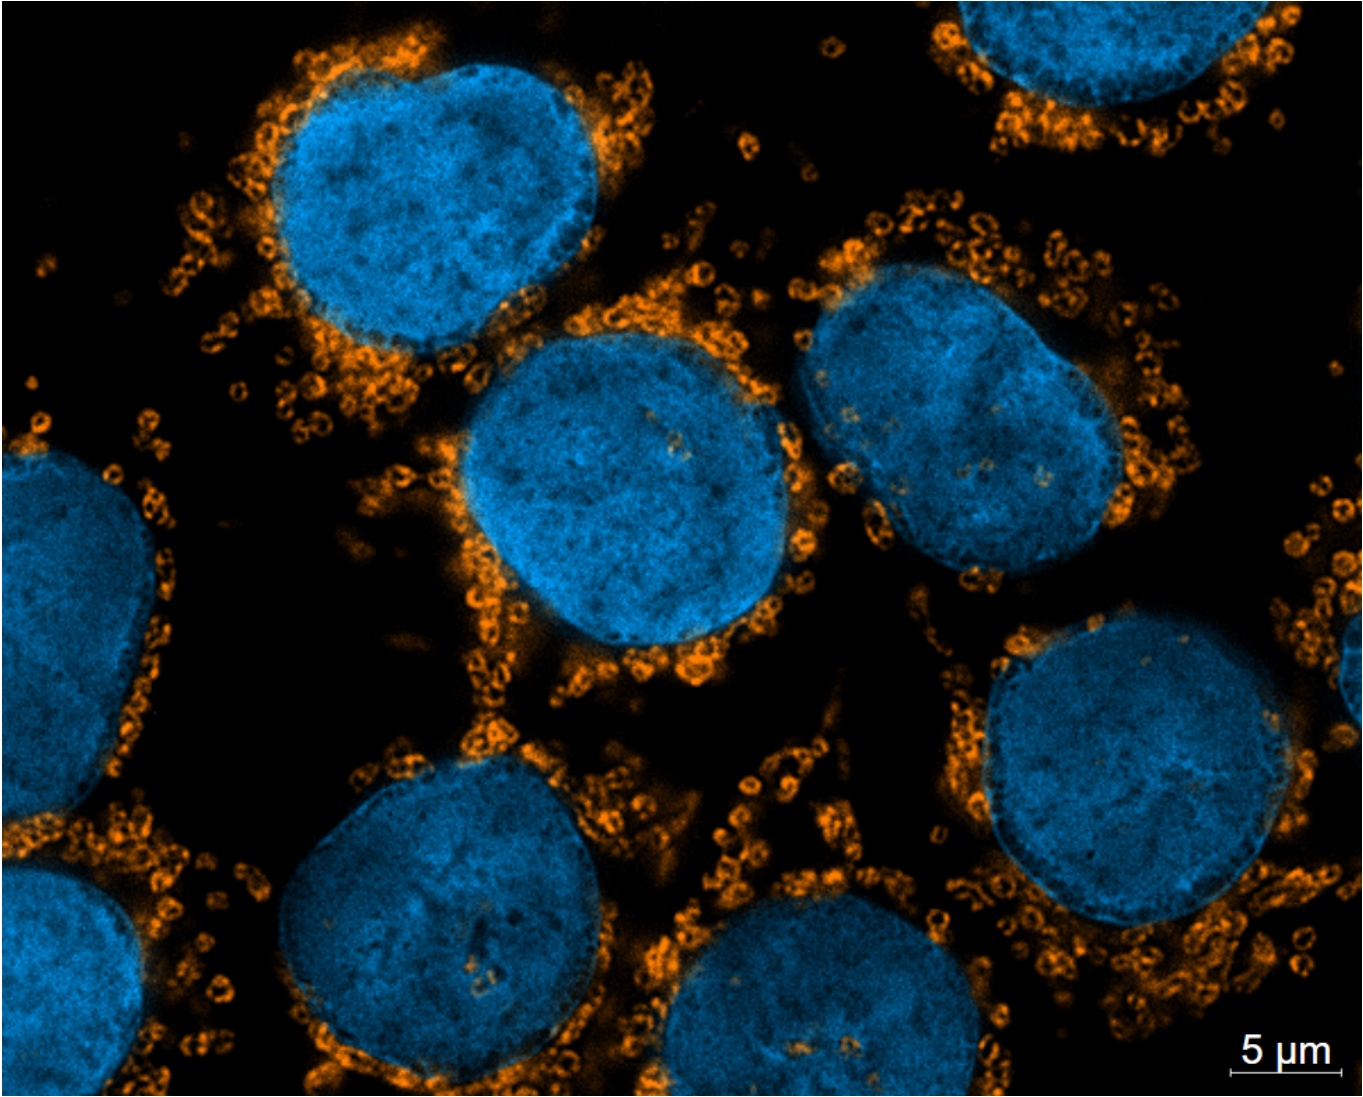

EVIDENCE TIER	Widefield
INSTRUMENT	ZEISS Axio Imager.M1
CELL MODEL	HCT116
DETECTED DYES	405/DAPI; 555
METADATA VALUES	30

STRUCTURED ACQUISITION METADATA / WIDEFIELD

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss Axio Imager.M1 Widefield, using a Plan-Apochromat 63x/1.40 Oil M27, Axiocam MR R3, and X-Cite Xylis Lamp was used with the following parameters for each dye:
Objective	Plan-Apochromat 63x/1.40 Oil M27
Channels	2
Scaling (Per Pixel)	0.102µm X 0.102µm
Image size (Pixels)	607 X 486
Image Size (Scaled)	62.15µm X 49.76µm
Bit Depth	12 Bit
Image Center Position	X: 0.00µm, Y: 0.00µm
ROI Center Offset	X: 0.00µm, Y: 0.00µm
Reflector	45 Texas Red 49 DAPI
Beam Splitter	585 395
Filter Excitation Wavelength	540 - 580 335 - 383
Filter Emission Wavelength	593 - 668 420 - 470
Contrast Method	Fluorescence
Light source	X-Cite Xylis Lamp Intensity @29% X-Cite Xylis Lamp Intensity @15%
Exposure Time	100ms 80ms
Excitation Wavelength	553 353
Emission Wavelength	568 465
Effective NA	1.4
Imaging Device	Axiocam MR R3
Camera Adapter	1X
Depth of Focus	0.88µm 0.72µm
Binning Mode	1,1

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit IgG (H + L)

Cat ID# - SA 000035

HCT 116 Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher Fish Serum Blocker cat#37527X3. The primary antibody, Mitochondria Rabbit Recombinant Antibody (MTC02,2860R), was incubated for 1 hour at room temperature at a dilution of 1:250. Cells were washed 3X in PBS, and Identifyn® 555 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss Axio Imager.M1 Widefield, using a Plan-Apochromat 63x/1.40 Oil M27, Axiocam MR R3, and X-Cite Xylis Lamp was used with the following parameters for each dye:

Single Plane (2D)

Channels = 2

Scaling (Per Pixel) = 0.102µm X 0.102µm

Image size (Pixels) = 607 X 486

Image Size (Scaled) = 62.15µm X 49.76µm

Bit Depth = 12 Bit

Image Center Position = X: 0.00µm, Y: 0.00µm

ROI Center Offset = X: 0.00µm, Y: 0.00µm

555 -

Reflector = 45 Texas Red

Beam Splitter = 585

Filter Excitation Wavelength = 540 - 580

Filter Emission Wavelength = 593 - 668

Contrast Method = Fluorescence

Light source = X-Cite Xylis Lamp Intensity @29%

Exposure Time = 100ms

Excitation Wavelength = 553

Emission Wavelength = 568

Effective NA = 1.4

Imaging Device = Axiocam MR R3

Camera Adapter = 1X

Depth of Focus = 0.88µm

Binning Mode = 1,1

DAPI -

Reflector = 49 DAPI
 Beam Splitter = 395
 Filter Excitation Wavelength = 335 - 383
 Filter Emission Wavelength = 420 - 470
 Contrast Method = Fluorescence
 Light source = X-Cite Xylis Lamp Intensity @15%
 Exposure Time = 80ms
 Excitation Wavelength = 353
 Emission Wavelength = 465
 Effective NA = 1.4
 Imaging Device = AxioCam MR R3
 Camera Adapter = 1X
 Depth of Focus = 0.72µm
 Binning Mode = 1,1

Post Processing

None

Image Correction

Unsharp Mask was used due to depth of field for the HCT116 Cells.


Image by E.F. Simon

Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE

Catalog	SA-000035
Stage	Widefield
Instrument	ZEISS Axio Imager.M1
Microscope configuration	Zeiss Axio Imager.M1 Widefield, using a Plan-Apochromat 63x/1.40 Oil M27, AxioCam MR R3, and X-Cite Xylis Lamp was used with the following parameters for each dye:
Structured source metadata values	30
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HCT116
Image SHA-256	33D68A3EB5C2CB5D1C0178E1059F1F3A4CA41A24906B6F8A1EC2D7B305A88637
Method PDF SHA-256	E20EDC60569006C4847C4A2371A57917469CE683B2093880FA8DDED27DCA516E

ORIGINAL IMAGE EVIDENCE / WIDEFIELD SIM - APOTOME

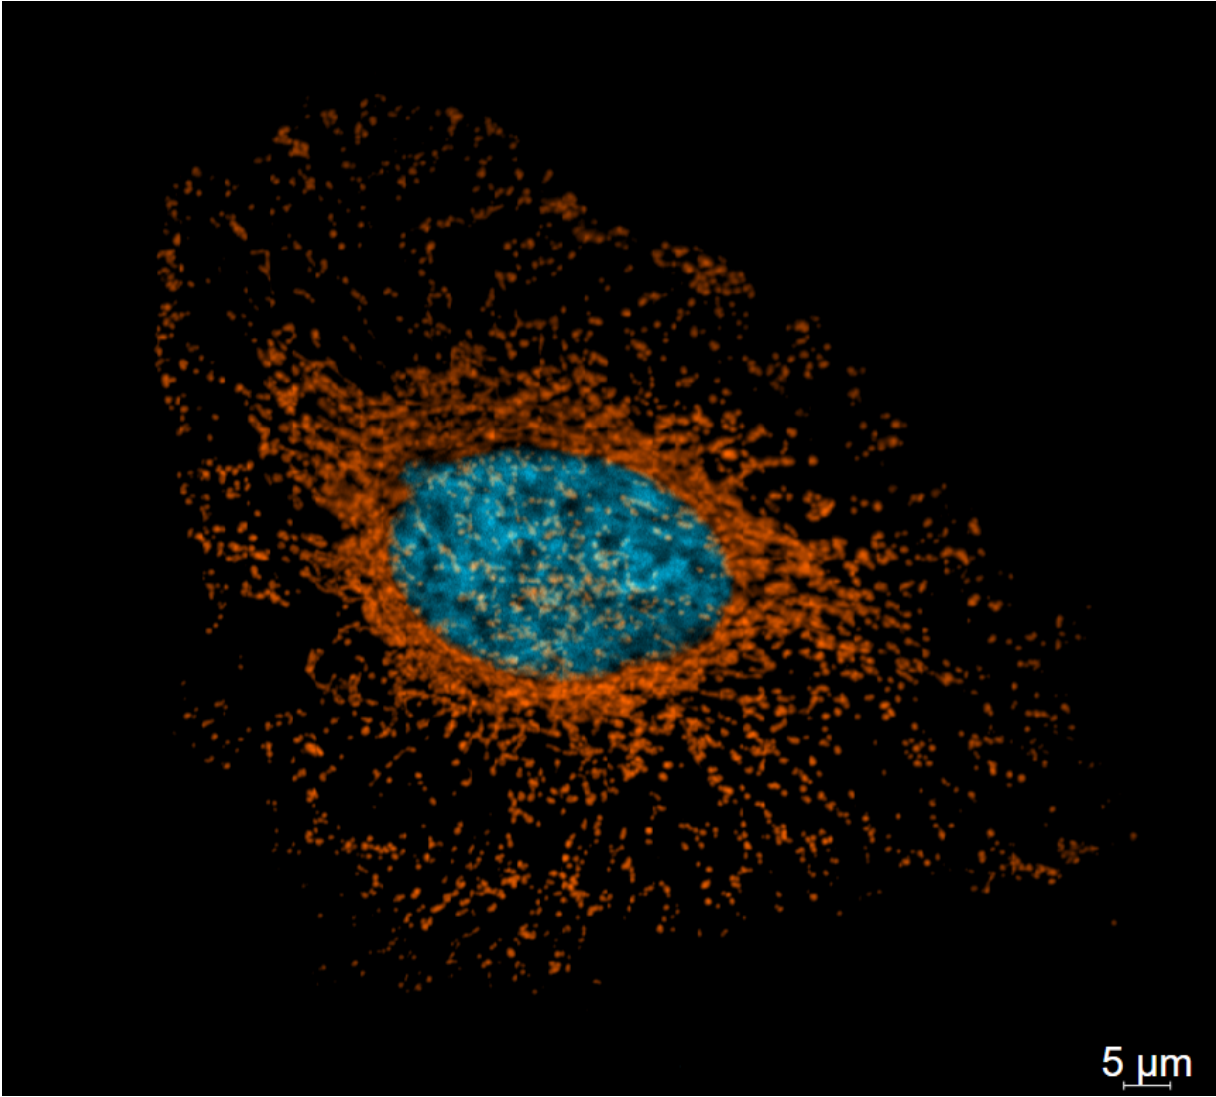

EVIDENCE TIER	Widefield SIM - Apotome
INSTRUMENT	ZEISS Axio Observer.Z1/7 Apotome
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 555
METADATA VALUES	32

STRUCTURED ACQUISITION METADATA / WIDEFIELD SIM - APOTOME

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:
Objective	EC Plan-Neofluar 63X/1.25 oil M27
Channels	2
Scaling (Per Pixel)	0.143µm X 0.143µm
Image Size (Pixels)	931 X 837
Image Size (Scaled)	133.07µm X 119.57µm
Bit Depth	14 Bit
Image Center Position	X: 45.29mm, Y:46.64mm
Stage Position	X: 45.29mm, Y:46.64mm
ROI Center Offset	X: 1.14µm, Y: 0.00µm
Reflector	45 Texas Red 49 DAPI
Beam Splitter	585 395
Filter Excitation Wavelength	540 - 580 335-383
Filter Emission Wavelength	593 - 668 420-470
Contrast Method	Fluorescence
Light source	X-Cite Xylis Lamp Intensity @37% X-Cite Xylis Lamp Intensity @5%
Exposure Time	120ms 40ms
Excitation Wavelength	553 353
Emission Wavelength	568 465
Effective NA	1.25
Imaging Device	Axiocam 807
Camera Adapter	1X
Depth of Focus	1.10µm 0.90µm
Binning Mode	2,2
Apotome SIM Image Processing	Display Mode "Optical Sectioning" - enabled correction selected.

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit IgG (H + L)

Cat ID# - SA 000035

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher Fish Serum Blocker cat#37527X3. The primary antibody, Mitochondria Rabbit Recombinant Antibody (MTC02,2860R), was incubated for 1 hour at room temperature at a dilution of 1:250. Cells were washed 3X in PBS, and Identifyn® 555 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:

Single Plane (2D)

Channels = 2

Scaling (Per Pixel) = 0.143µm X 0.143µm

Image Size (Pixels) = 931 X 837

Image Size (Scaled) = 133.07µm X 119.57µm

Bit Depth = 14 Bit

Image Center Position = X: 45.29mm, Y:46.64mm

Stage Position = X: 45.29mm, Y:46.64mm

ROI Center Offset = X: 1.14µm, Y: 0.00µm

555 -

Reflector = 45 Texas Red

Beam Splitter = 585

Filter Excitation Wavelength = 540 - 580

Filter Emission Wavelength = 593 - 668

Contrast Method = Fluorescence

Light source = X-Cite Xylis Lamp Intensity @37%

Exposure Time = 120ms

Excitation Wavelength = 553

Emission Wavelength = 568

Effective NA = 1.25

Imaging Device = Axiocam 807

Camera Adapter = 1X

Depth of Focus = 1.10µm

Binning Mode = 2,2

DAPI -

Reflector = 49 DAPI
 Beam Splitter = 395
 Filter Excitation Wavelength = 335-383
 Filter Emission Wavelength = 420-470
 Contrast Method = Fluorescence
 Light source = X-Cite Xylis Lamp Intensity @5%
 Exposure Time = 40ms
 Excitation Wavelength = 353
 Emission Wavelength = 465
 Effective NA = 1.25
 Imaging Device = Axiocam 807
 Camera Adapter = 1X
 Depth of Focus = 0.90µm
 Binning Mode = 2,2

Post Processing - SIM Processing

Apotome SIM Image Processing = Display Mode "Optical Sectioning" - enabled correction selected.
 Normalization, Phase Corrector, Fourier Filter, and Deconvolution were NOT used.

Image Corrections


None

Image by E.F Simon

Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE	
Catalog	SA-000035
Stage	Widefield SIM - Apotome
Instrument	ZEISS Axio Observer.Z1/7 Apotome
Microscope configuration	Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:
Structured source metadata values	32
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	1E2E73523EE112CDAB05918B6E94B8E82EE5FECAC84D83695403EF78235376D0
Method PDF SHA-256	951E4B2E0B2161EB7D9A7D172ECA4414A79AC072CC3C0E8768FCF19735F8536C

ORIGINAL IMAGE EVIDENCE / CONFOCAL

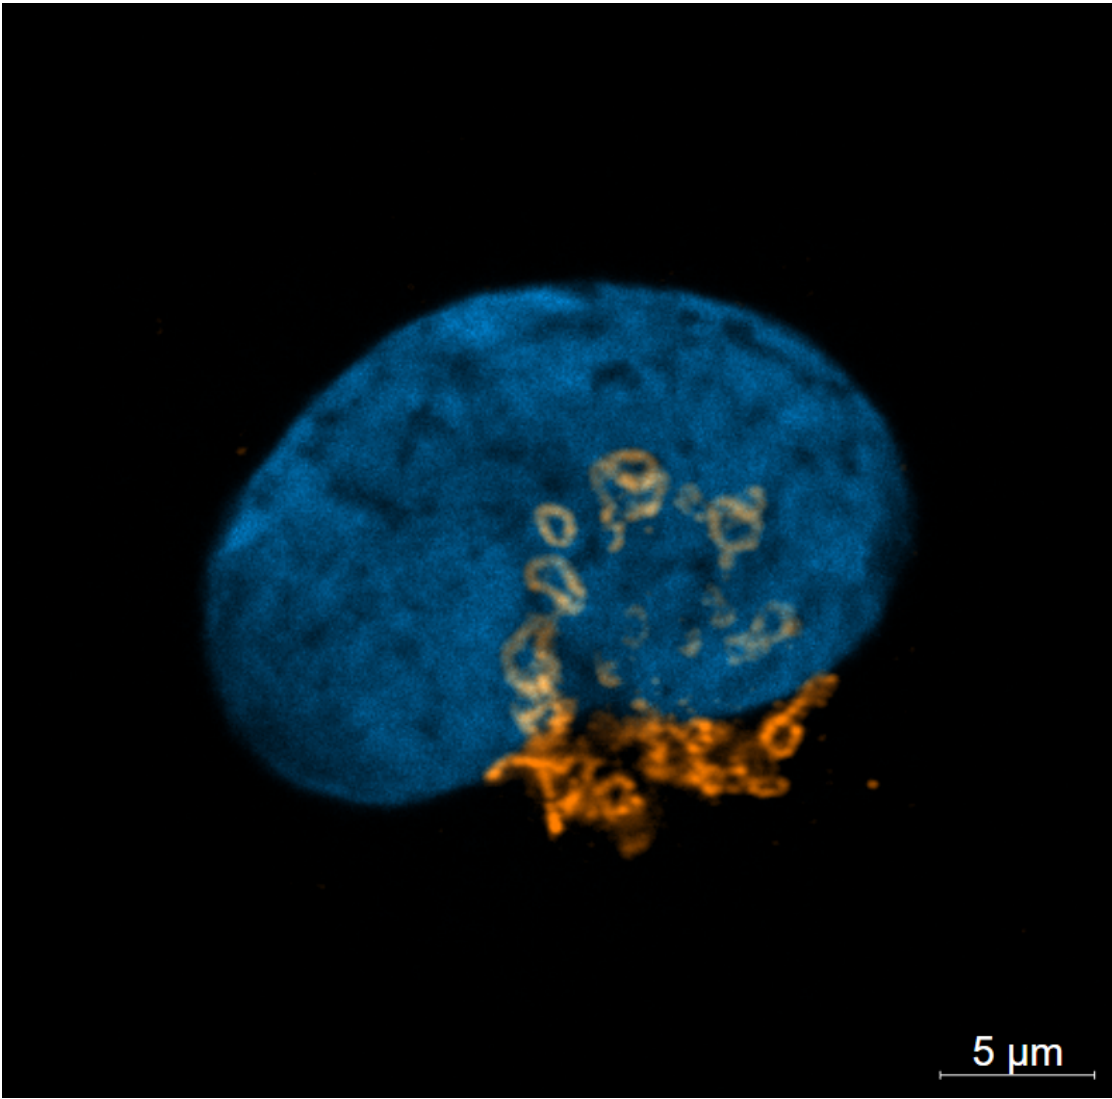

EVIDENCE TIER	Confocal
INSTRUMENT	ZEISS LSM 900
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 488; 555
METADATA VALUES	38

STRUCTURED ACQUISITION METADATA / CONFOCAL

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss LSM 900 Confocal, Axio Observer.Z1/7, using with a Plan-Apochromat 63X/1.40 oil DIC M27 was used with the following parameters for each dye:
Objective	with a Plan-Apochromat 63X/1.40 oil DIC M27
Channels	2
Scaling (Per Pixel)	0.071µm X 0.071µm
Image size (Pixels)	523 X 509
Image Size (Scaled)	36.92µm X 35.94µm
Bit Depth	16 Bit
Image Center Position	X: 65.91mm, Y: 49.26mm
Stage Position	X: 65.91mm, Y: 49.26mm
ROI Center Offset	X: 0.00µm, Y: 0.00µm
Reflector	None
Contrast Method	Fluorescence
Pinhole	1.00AU / 49µm 1.00AU / 37µm
LMS MBS	MBS 405 + 488 + 561 + 640(T10/R90)
Laser Wavelength	561nm @1.0% 405nm @0.7%
Laser Blanking	Enabled
Scan Mode	Frame
Scan Zoom	1.4
Rotation	0°
Sampling	1.00
Pixel Time	0.51µs
Frame Time	10.15s
LSM Scan Speed	9
Scan Direction	Bidirectional
Line Step	1
Excitation Wavelength	553 353
Emission Wavelength	568 465
Effective NA	1.4
Detection Wavelength	545 - 610 410 - 470
Imaging Device	Airyscan
Detector Type	GaAsP-PMT
Detector Gain	650 V
Detector Offset	0

FIELD	SOURCE-DOCUMENTED VALUE
Detector Digital Gain	1.0
The histogram was adjusted to the following	Black 52, Gamma 1.16, White 23171

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit IgG (H + L)

Cat ID# - SA 000035

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher Fish Serum Blocker cat#37527X3. The primary antibody, Golgi GOLPH2 Polyclonal Antibody, was incubated for 1 hour at room temperature at a dilution of 1:250. Cells were washed 3X in PBS, and Identifyn® 555 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss LSM 900 Confocal, Axio Observer.Z1/7, using with a Plan-Apochromat 63X/1.40 oil DIC M27 was used with the following parameters for each dye:

Single Plane (2D)

Channels = 2

Scaling (Per Pixel) = 0.071µm X 0.071µm

Image size (Pixels) = 523 X 509

Image Size (Scaled) = 36.92µm X 35.94µm

Bit Depth = 16 Bit

Image Center Position = X: 65.91mm, Y: 49.26mm

Stage Position = X: 65.91mm, Y: 49.26mm

ROI Center Offset = X: 0.00µm, Y: 0.00µm

555 -

Reflector = None
 Contrast Method = Fluorescence
 Pinhole = 1.00AU / 49µm
 LMS MBS = MBS 405 + 488 + 561 + 640(T10/R90)
 Laser Wavelength = 561nm @1.0%
 Laser Blanking = Enabled
 Scan Mode = Frame
 Scan Zoom = 1.4
 Rotation = 0°
 Sampling = 1.00
 Pixel Time = 0.51µs
 Frame Time = 10.15s
 LSM Scan Speed = 9
 Scan Direction = Bidirectional
 Line Step = 1
 Averaging - 16
 Excitation Wavelength = 553
 Emission Wavelength = 568
 Effective NA = 1.4
 Detection Wavelength = 545 - 610
 Imaging Device = Airyscan
 Detector Type = GaAsp-PMT
 Detector Gain = 650 V
 Detector Offset = 0
 Detector Digital Gain = 1.0

DAPI -

Reflector = None
 Contrast Method = Fluorescence
 Pinhole = 1.00AU / 37µm
 LMS MBS = MBS 405 + 488 + 561 + 640(T10/R90)
 Laser Wavelength = 405nm @0.7%
 Laser Blanking = Enabled
 Scan Mode = Frame
 Scan Zoom = 1.4
 Rotation = 0°
 Sampling = 1.00
 Pixel Time = 0.51µs
 Frame Time = 10.15s
 LSM Scan Speed = 9
 Scan Direction = Bidirectional
 Line Step = 1
 Averaging - 16
 Excitation Wavelength = 353
 Emission Wavelength = 465
 Effective NA = 1.4
 Detection Wavelength = 410 - 470
 Imaging Device = Airyscan
 Detector Type = GaAsP-PMT
 Detector Gain = 650 V
 Detector Offset = 0
 Detector Digital Gain = 1.0

Post Processing

N/A

Image Corrections

DAPI was corrected to reduce signal brightness as colocalization at the 555 (Golgi staining) was reducing image clarity in the presentation of the 555 signal.

Best Fit was selected at 2.00 and 0.01 (Spline Mode)

The histogram was adjusted to the following = Black 52, Gamma 1.16, White 23171

Image by J.K. Bennett

Copyright 2026 GMD12 LLC.


SOURCE PROVENANCE

Catalog	SA-000035
Stage	Confocal
Instrument	ZEISS LSM 900

SOURCE PROVENANCE

Microscope configuration	Zeiss LSM 900 Confocal, Axio Observer.Z1/7, using with a Plan-Apochromat 63X/1.40 oil DIC M27 was used with the following parameters for each dye:
Structured source metadata values	38
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	112511DE3E09718E0856043601B496624415C0E83268C37D4AC6470ABAE9A2A0
Method PDF SHA-256	73A3946419A8528806955096D75F69AA1EA1721F34A04AD8B5A48FD469FD2E5E

ORIGINAL IMAGE EVIDENCE / AIRYSCAN

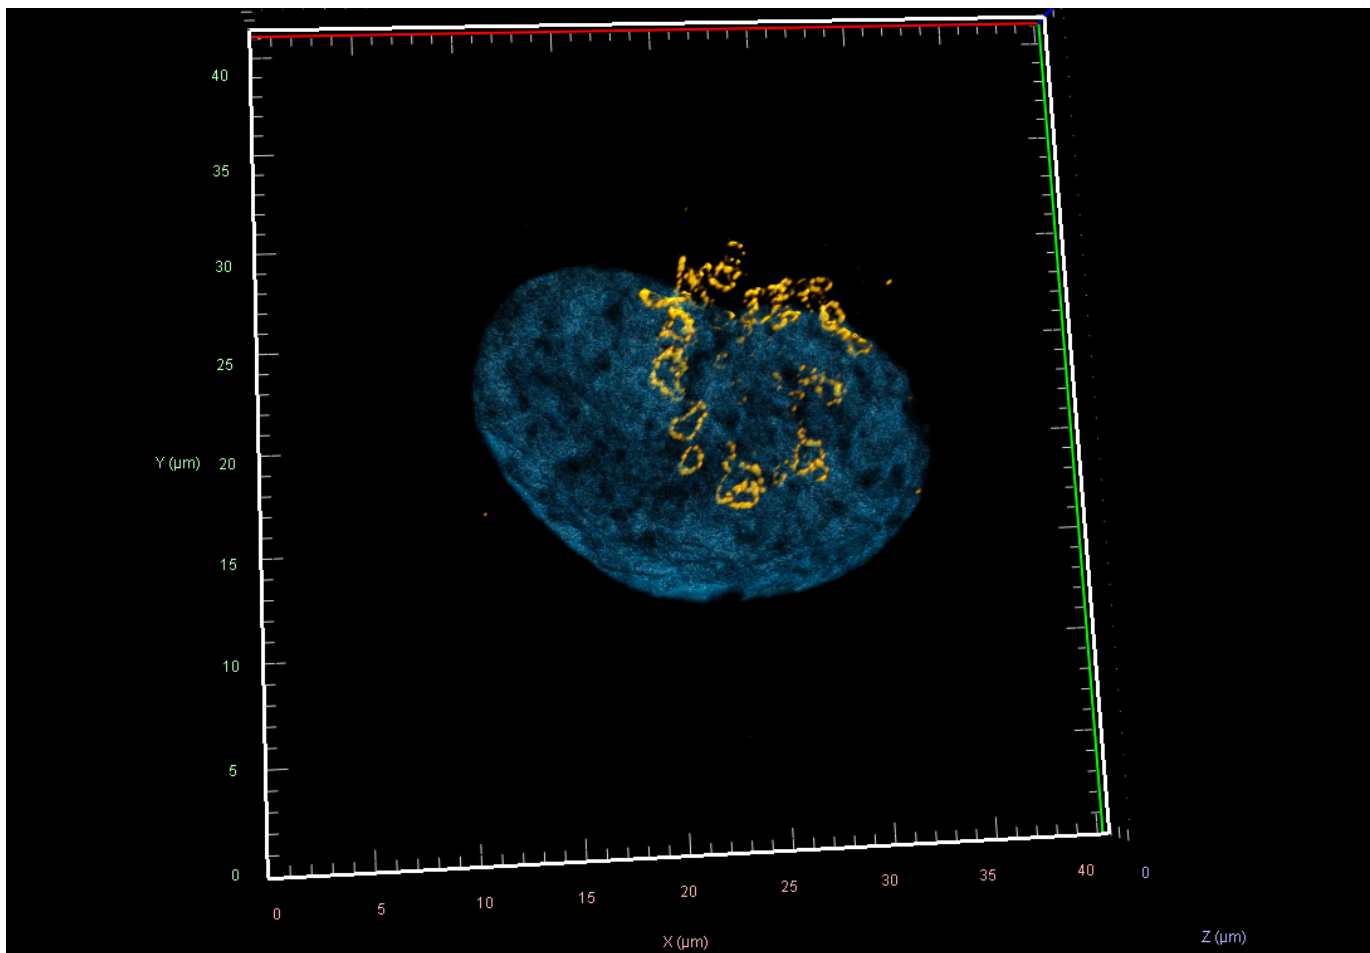

EVIDENCE TIER	Airyscan
INSTRUMENT	ZEISS LSM 900
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 488; 555
METADATA VALUES	50

STRUCTURED ACQUISITION METADATA / AIRYSCAN

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss LSM 900 Confocal, Axio Observer.Z1/7, using with a Plan-Apochromat 63X/1.40 oil DIC M27 was used with the following parameters for each dye:
Objective	with a Plan-Apochromat 63X/1.40 oil DIC M27
Z-Stack	65 Slices (3.20µm)
Channels	2
Scaling (Per Pixel)	0.03529 µm X 0.03529 µm X 0.05000 µm
Image Size (Pixels)	1141 X 1165
Image Size (Scaled)	40.26µm X 41.11µm
Bit Depth	16 Bit
Image Center Position	X: 65.91mm, Y: 49.26mm
Stage Position	X: 65.91mm, Y: 49.26mm
ROI Center Offset	X: 0.00µm, Y: 0.00µm
Reflector	None
Contrast Method	Fluorescence
Pinhole	5.00AU / 245µm 5.00AU / 188µm
LMS MBS	MBS 405 + 488 + 561 + 640(T10/R90)
Laser Wavelength	561nm @0.5% 405nm @0.5%
Laser Blanking	Enabled
Scan Mode	Frame
Scan Zoom	1.5
Rotation	0°
Sampling	2.00
Pixel Time	0.55µs
Frame Time	9.48s
LSM Scan Speed	7
Scan Direction	Bidirectional
Line Step	1
Excitation Wavelength	553 353
Emission Wavelength	568 465
Effective NA	1.4
Detection Wavelength	550 - 610 400 - 495
Imaging Device	Airyscan
Detector Type	GaAsp-PMT
Detector Gain	800 V

FIELD	SOURCE-DOCUMENTED VALUE
Detector Offset	0
Detector Digital Gain	1.0
AiryScan Mode	Super Resolution 10.0 (3D, Auto) Super Resolution 8.8 (3D, Auto)
3D Volume Projection	Precise
Appearance	Threshold 0%, Ramp 98%, Maximum 100%
Background	Black
Light	Brightness148%, Azimuth 80°, Elongation -130°, Enabled Directional Lighting, Enabled Tone Mapping
Projection	View Angle 35°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)
Clipping Image Process	Clipping planes are introduced to pronounce regions of special interest.
X - Y	Active was selected, Invisible was chosen to remove the obstruction from the image below the cut plane, and a White Outline of the clipped perimeter was shown; Clip Back was Selected, and Clip Front was NOT selected.
Position of Clip	-36%
Clip X	0°
Clip Y	0°

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit IgG (H + L)

Cat ID# - SA 000035

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher, Fish Serum Blocker cat#37527X3. The primary antibody, Golgi GOLPH2 Polyclonal Antibody, was incubated overnight at 4°C at a dilution of 1:100. Cells were washed 3X in PBS. Identifyn® 555 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss LSM 900 Confocal, Axio Observer.Z1/7, using with a Plan-Apochromat 63X/1.40 oil DIC M27 was used with the following parameters for each dye:

Z Stack - (3D)

Z-Stack = 65 Slices (3.20µm)

Channels = 2

Scaling (Per Pixel) = 35.29nm X 35.29nm X 50.00nm

Image Size (Pixels) = 1141 X 1165

Image Size (Scaled) = 40.26µm X 41.11µm

Bit Depth = 16 Bit

Image Center Position = X: 65.91mm, Y: 49.26mm

Stage Position = X: 65.91mm, Y: 49.26mm

ROI Center Offset = X: 0.00µm, Y: 0.00µm

555 -

Reflector = None
 Contrast Method = Fluorescence
 Pinhole = 5.00AU / 245µm
 LMS MBS = MBS 405 + 488 + 561 + 640(T10/R90)
 Laser Wavelength = 561nm @0.5%
 Laser Blanking = Enabled
 Scan Mode = Frame
 Scan Zoom = 1.5
 Rotation = 0°
 Sampling = 2.00
 Pixel Time = 0.55µs
 Frame Time = 9.48s
 LSM Scan Speed = 7
 Scan Direction = Bidirectional
 Line Step = 1
 Averaging - 4
 Excitation Wavelength = 553
 Emission Wavelength = 568
 Effective NA = 1.4
 Detection Wavelength = 550 - 610
 Imaging Device = Airyscan
 Detector Type = GaAsP-PMT
 Detector Gain = 800 V
 Detector Offset = 0
 Detector Digital Gain = 1.0
 AiryScan Mode = Super Resolution 10.0 (3D, Auto)

DAPI -

Reflector = None
 Contrast Method = Fluorescence
 Pinhole = 5.00AU / 188µm
 LMS MBS = MBS 405 + 488 + 561 + 640(T10/R90)
 Laser Wavelength = 405nm @0.5%
 Laser Blanking = Enabled
 Scan Mode = Frame
 Scan Zoom = 1.5
 Rotation = 0°
 Sampling = 2.00
 Pixel Time = 0.55µs
 Frame Time = 9.48s
 LSM Scan Speed = 7
 Scan Direction = Bidirectional
 Line Step = 1
 Averaging - 4
 Excitation Wavelength = 353
 Emission Wavelength = 465
 Effective NA = 1.4
 Detection Wavelength = 400 - 495
 Imaging Device = Airyscan
 Detector Type = GaAsP-PMT
 Detector Gain = 800 V
 Detector Offset = 0
 Detector Digital Gain = 1.0
 AiryScan Mode = Super Resolution 8.8 (3D, Auto)

3D Image Processing

3D Volume Projection = Precise
 Appearance = Threshold 0%, Ramp 98%, Maximum 100%
 Background = Black
 Light = Brightness 148%, Azimuth 80°, Elongation -130°, Enabled Directional Lighting, Enabled Tone Mapping
 Projection = View Angle 35°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)
 Clipping Image Process = Clipping planes are introduced to pronounce regions of special interest.
 X - Y = Active was selected, Invisible was chosen to remove the obstruction from the image below the cut plane, and a White Outline of the clipped perimeter was shown; Clip Back was Selected, and Clip Front was NOT selected.
 Position of Clip = -36%
 Clip X = 0°
 Clip Y = 0°

Image Corrections

None

Image by J.K. Bennett


Copyright 2026 GMD12 LLC.

Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE

Catalog	SA-000035
Stage	Airyscan
Instrument	ZEISS LSM 900
Microscope configuration	Zeiss LSM 900 Confocal, Axio Observer.Z1/7, using with a Plan-Apochromat 63X/1.40 oil DIC M27 was used with the following parameters for each dye:
Structured source metadata values	50
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	3197C0A78DD5F00075755E59C93C29F7F52065217CC911907A545C4CD05C9D20
Method PDF SHA-256	C34750D675D2F7659479E595591D72275D37B194E4304F5971F9C45D3764BEF3

ORIGINAL IMAGE EVIDENCE / SIM

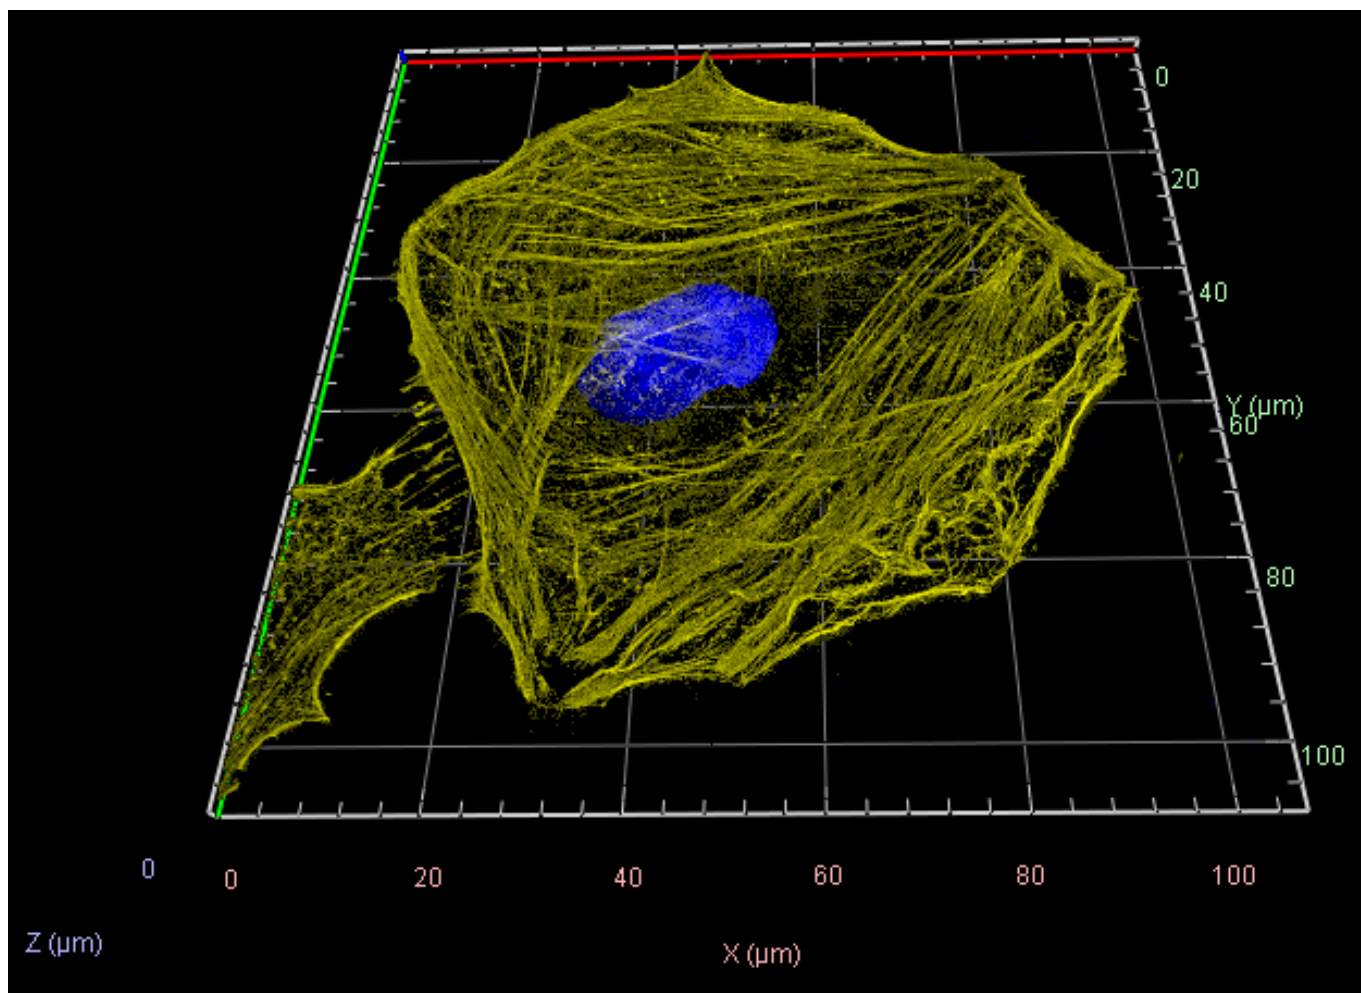

EVIDENCE TIER	SIM
INSTRUMENT	ZEISS Elyra
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 488; 555
METADATA VALUES	54

STRUCTURED ACQUISITION METADATA / SIM

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss Elyra 5 Lattice SIM, AxioObserver.Z1/ 7 using Plan-Apochromat 63X/1.40 oil DIC M27, 1X Tubelens, was used with the following parameters for each dye:
Objective	Plan-Apochromat 63X/1.40 oil DIC M27
Z-Stack	39 Slices (1.9µm)
Channels	2 1
Scaling (Per Pixel)	0.04223 µm X 0.04223 µm X 0.05000 µm
Image Size (Pixels)	2528 X 2528
Image Size (Scaled)	106.75µm X 106.75µm
Bit Depth	16 Bit
Image Center Position	X: 61.84mm, Y: 35.09mm
Stage Position	X: 61.84mm, Y: 35.09mm
ROI Center Offset	X: 0.00µm, Y: 0.00µm
Reflectors	SR HE LBF 405/488/561/642
Beam Splitter	405, 488, 561, 642
Filter Excitation Wavelength	200 - 405, 200 - 488, 200 - 561, 200 - 642
Filter Emission Wavelength	419 - 470, 503 - 546, 576 - 617, 657 - 800
Contrast Method	Fluorescence
Illumination Wavelength	561 405
Channel Name	T2-Axiocam 820 #2-SR
Excitation Wavelength	561 405
Emission Wavelength	583 525
Effective NA	1.4
Detection Wavelength	503 - 546, 576 - 590
Imaging Device	Axiocam 820#2
Camera Adapter	1X
Exposure Time	75ms 50ms
Depth of Focus	0.90µm 0.81µm
Binning Mode	2,2
Laser Wavelength	561nm @0.5% 405nm @1.0%
Frame Time	1.33s 676.00ms
Scan Direction	Unidirectional
Result Sampling	2
Process Sampling	2
Algorithm	SIM

FIELD	SOURCE-DOCUMENTED VALUE
SIM Settings	Standard
Auto Sharpness	On
Sharpness	11.3211
Input SNR	N/A
Regularization Weight	N/A
Iterations	N/A
Filter	N/A
Fitting	N/a
Normalization	Automatic
Experimental PSF	N/A
3D Maximum Projection	Precise
Appearance	Threshold 4% (555), Threshold 4% (405) Ramp 0% all channels, Maximum 100% all channels
Background	Black
Light	Brightness 119%, Enabled Tone Mapping
Projection	View Angle 61°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit IgG (H + L)

Cat ID# - SA 000035

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher Fish Serum Blocker cat#37527X3. The primary antibody, Actin Monoclonal Antibody (mAbGEa), was incubated for 1 hour at room temperature at a dilution of 1:250. Cells were washed 3X in PBS, and Identifyn® 555 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss Elyra 5 Lattice SIM, AxioObserver.Z1/ 7 using Plan-Apochromat 63X/1.40 oil DIC M27, 1X Tubelens, was used with the following parameters for each dye:

Z Stack - (3D)

Z-Stack = 39 Slices (1.9µm)

Channels = 2

Scaling (Per Pixel) = 42.23nm X 42.23nm X 50.00nm

Image Size (Pixels) = 2528 X 2528

Image Size (Scaled) = 106.75µm X 106.75µm

Bit Depth = 16 Bit

Image Center Position = X: 61.84mm, Y: 35.09mm

Stage Position = X: 61.84mm, Y: 35.09mm

ROI Center Offset = X: 0.00µm, Y: 0.00µm

555 -

Reflectors = SR HE LBF 405/488/561/642
 Beam Splitter = 405, 488, 561, 642
 Filter Excitation Wavelength = 200 - 405, 200 - 488, 200 - 561, 200 - 642
 Filter Emission Wavelength = 419 - 470, 503 - 546, 576 - 617, 657 - 800
 Contrast Method = Fluorescence
 Illumination Wavelength = 561
 Channel Name = T2-Axiocam 820 #2-SR
 Excitation Wavelength = 561
 Emission Wavelength = 583
 Effective NA = 1.4
 Detection Wavelength = 503 - 546, 576 - 590
 Imaging Device = Axiocam 820#2
 Camera Adapter = 1X
 Exposure Time = 75ms
 Depth of Focus = 0.90µm
 Binning Mode = 2,2
 Laser Wavelength = 561nm @0.5%
 Frame Time = 1.33s
 Scan Direction = Unidirectional
 Grating 27.5µm grating

DAPI -

Reflectors = SR HE LBF 405/488/561/642
 Beam Splitter = 405, 488, 561, 642
 Filter Excitation Wavelength = 200 - 405, 200 - 488, 200 - 561, 200 - 642
 Filter Emission Wavelength = 419 - 470, 503 - 546, 576 - 617, 657 - 800
 Contrast Method = Fluorescence
 Illumination Wavelength = 405
 Channel Name = T2-Axiocam 820 #2-SR
 Excitation Wavelength = 405
 Emission Wavelength = 525
 Effective NA = 1.4
 Detection Wavelength = 503 - 546, 576 - 590
 Imaging Device = Axiocam 820#2
 Camera Adapter = 1X
 Exposure Time = 50ms
 Depth of Focus = 0.81µm
 Binning Mode = 2,2
 Laser Wavelength = 405nm @1.0%
 Frame Time = 676.00ms
 Scan Direction = Unidirectional
 Grating 36.5µm grating

Post Processing - SIM Processing

Processing Dimension - 3D
 Result Sampling = 2
 Process Sampling = 2
 Channels = 1
 Algorithm = SIM
 SIM Settings = Standard
 Auto Sharpness = On
 Sharpness = 11.3211
 Input SNR = N/A
 Regularization Weight = N/A
 Iterations = N/A
 Filter = N/A
 Fitting = N/a
 Normalization = Automatic
 Experimental PSF = N/A

3D Image Processing

3D Maximum Projection = Precise
 Appearance = Threshold 4% (555), Threshold 4% (405) Ramp 0% all channels, Maximum 100% all channels
 Background = Black
 Light = Brightness 119%, Enabled Tone Mapping
 Projection = View Angle 61°, Scale Z 100%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

Image Corrections

None

Image by P. Raut

Copyright 2026 GMD12 LLC.


SOURCE PROVENANCE	
Catalog	SA-000035
Stage	SIM
Instrument	ZEISS Elyra
Microscope configuration	Zeiss Elyra 5 Lattice SIM, AxioObserver.Z1/ 7 using Plan-Apochromat 63X/1.40 oil DIC M27, 1X Tubelens, was used with the following parameters for each dye:
Structured source metadata values	54
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	021CDB05A65B76089A9207A13C3F4401B27B428E616446E23FEDAB2CA33FC636

SOURCE PROVENANCE

Method PDF SHA-256

45E1E4C2FF02E8A606CE57F41CD3A7B8AA9BDC27201C0880AE8286223279761D

ORIGINAL IMAGE EVIDENCE / SIM²

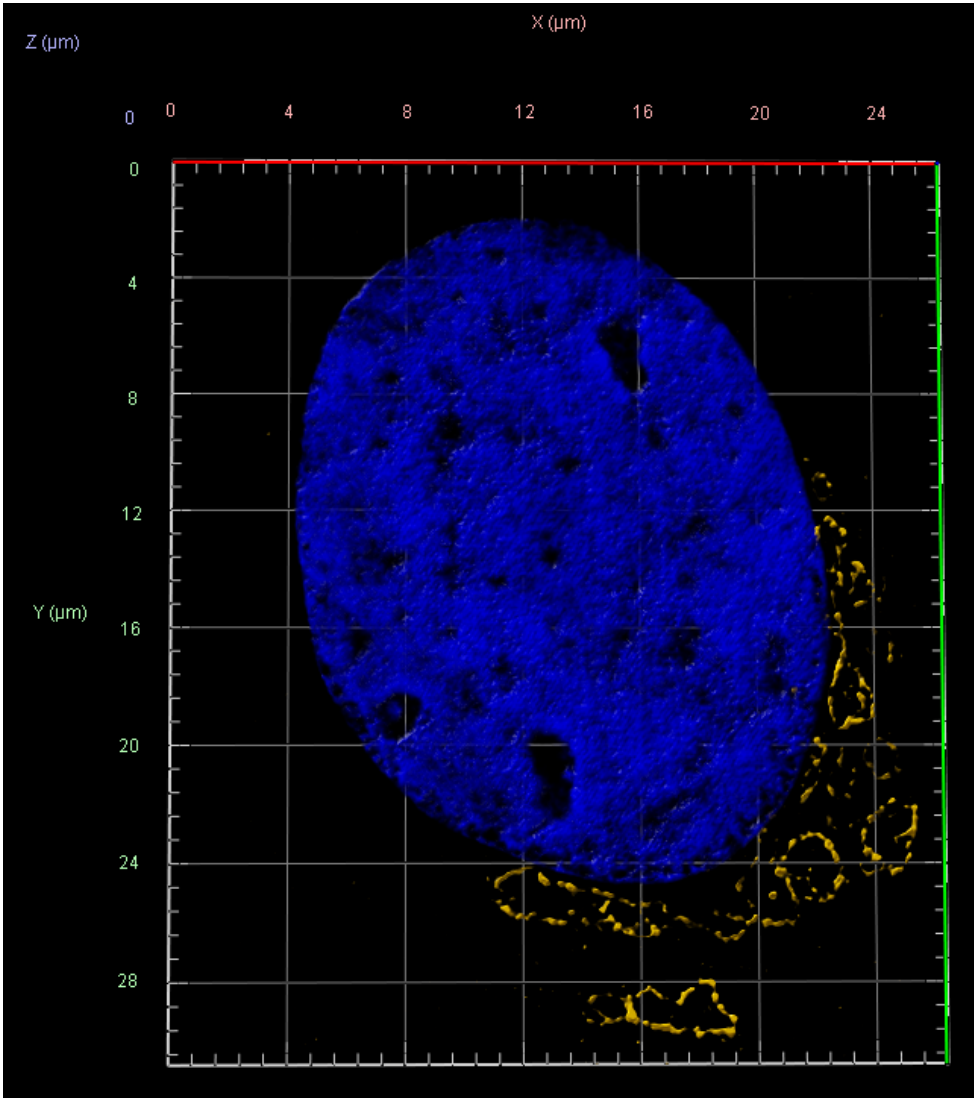

EVIDENCE TIER	SIM ²
INSTRUMENT	ZEISS Elyra 7
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 488; 555
METADATA VALUES	62

STRUCTURED ACQUISITION METADATA / SIM²

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss Elyra 7, Andor1, AxioObserver, using Plan-Apochromat 63X/1.46 oil Korr M27 was used with the following parameters for each dye:
Objective	Plan-Apochromat 63X/1.46 oil Korr M27
Filters	-2147483648
Beam Splitter 555	Main Beam Splitter Non-Descanned: LBF 405/488/561/642
Dual Camera Beam Splitter	SBS LP 640
Beam Splitter 405	Main Beam Splitter Non-Descanned: LBF 405/488/561/642
Calibration Marker Positions	Marker 1: 0.00µm, 0.00µm, Marker 2: 0.00µm, 0.00µm, Marker 3 0.00µm, 0.00µm
Z-Stack	6 Slices (350nm)
Channels	2
Scaling (Per Pixel)	0.01565 µm X 0.01565 µm X 58.33333 µm
Image Size (Pixels)	1683 X 1965
Image Size (Scaled)	26.34µm X 30.76µm
Bit Depth	16 Bit
Image Center Position	X: 136.60mm, Y: 5.42mm
Stage Position	X: 136.60mm, Y: 5.42mm
ROI Center Offset	X: 0.00µm, Y: 0.00µm
Contrast Method	Fluorescence
Laser Wavelength	642nm @10.0% 405nm @10.0%
Scan Mode	Other
Scan Zoom	1.0
Rotation	0°
Frame Time	1.0s
Scan Direction	Unidirectional
Line Step	N/A
Averaging	16
Excitation Wavelength	642 405
Emission Wavelength	655 515
Effective NA	1.46
Imaging Device	Edge 4.2 SIM
Exposure Time	120ms 100ms
Depth of Focus	0.93µm 0.73µm
Binning Mode	1x1
Detector Type	Camera

FIELD	SOURCE-DOCUMENTED VALUE
Depth Offset	0
Detector Digital Gain	0.00
Channel	561.000000 405.000000
Grating Period (µm)	27.500000 36.500000
Processing	3D
Input SNR	Medium Low
Iterations	16 5
Regularization Weight	0.0650000 0.800000
Processing Sampling	4
Output Sampling	4
Filter	Median
Detrend	No
Sectioning	100.000000
Baseline	Yes
Scale to Raw Image	No
Experimental PSF	No
3D Volume Projection	Precise
Appearance	Threshold 9% (555), Threshold 3% (405), Ramp 91% (555), Ramp 97% (405), Maximum 100% both channels
Background	Black
Light	Brightness 152%, Azimuth 25°, Elongation 131°, Enabled Directional Lighting, Enabled Tone Mapping
Projection	View Angle 35°, Scale Z 51%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

SOURCE METHOD

The text below is carried from the preserved Identifyfyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyfyn Standards for Optical Microscopy Methods™

Identifyfyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit IgG (H + L)

Cat ID# - SA 000035

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher Fish Serum Blocker cat#37527X3. The primary antibody, Golgi GOLPH2 Polyclonal Antibody, was incubated for 1 hour at room temperature at a dilution of 1:250. Cells were washed 3X in PBS, and Identifyfyn® 555 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss Elyra 7, Andor1, AxioObserver, using Plan-Apochromat 63X/1.46 oil Korr M27 was used with the following parameters for each dye:

Filters = -2147483648

Beam Splitter 555 = Main Beam Splitter Non-Descanned: LBF 405/488/561/642

Dual Camera Beam Splitter = SBS LP 640

Beam Splitter 405 = Main Beam Splitter Non-Descanned: LBF 405/488/561/642

Dual Camera Beam Splitter = SBS LP 640

Calibration Marker Positions: Marker 1: 0.00µm, 0.00µm, Marker 2: 0.00µm, 0.00µm, Marker 3 0.00µm, 0.00µm

Z Stack - (3D)

Z-Stack = 6 Slices (350nm)

Channels = 2

Scaling (Per Pixel) = 15.65nm X 15.65nm X 70.00nm

Image Size (Pixels) = 1683 X 1965

Image Size (Scaled) = 26.34µm X 30.76µm

Bit Depth = 16 Bit

Image Center Position = X: 136.60mm, Y: 5.42mm

Stage Position =X: 136.60mm, Y: 5.42mm

ROI Center Offset = X: 0.00µm, Y: 0.00µm

555 -

Contrast Method = Fluorescence
 Laser Wavelength = 642nm @10.0%
 Scan Mode = Other
 Scan Zoom = 1.0
 Rotation = 0°
 Frame Time = 1.0s
 Scan Direction = Unidirectional
 Line Step = N/A
 Averaging = 16
 Excitation Wavelength = 642
 Emission Wavelength = 655
 Effective NA = 1.46
 Imaging Device = Edge 4.2 SIM
 Exposure Time = 120ms
 Depth of Focus = 0.93µm
 Binning Mode = 1x1
 Detector Type = Camera
 Depth Offset = 0
 Detector Digital Gain = 0.00

Post Processing - SIM2 Processing

Channel = 561.000000
Grating Period (µm): 27.500000

SIM2

Processing: 3D
 Input SNR: Medium
 Iterations: 16
 Regularization Weight: 0.0650000
 Processing Sampling: 4
 Output Sampling: 4
 Filter: Median
 Detrend: No
 Sectioning: 100.000000
 Baseline: Yes
 Scale to Raw Image: No
 Experimental PSF: No

DAPI -

Contrast Method = Fluorescence
 Laser Wavelength = 405nm @10.0%
 Scan Mode = Other
 Scan Zoom = 1.0
 Rotation = 0°
 Frame Time = 1.0s
 Scan Direction = Unidirectional
 Line Step = N/A
 Averaging = 16
 Excitation Wavelength = 405
 Emission Wavelength = 515
 Effective NA = 1.46
 Imaging Device = Edge 4.2 SIM
 Exposure Time = 100ms
 Depth of Focus = 0.73µm
 Binning Mode = 1x1
 Detector Type = Camera
 Depth Offset = 0
 Detector Digital Gain = 0.00

Post Processing - SIM2 Processing

Channel = 405.000000
Grating Period (µm): 36.500000

SIM2

Processing: 3D
 Input SNR: Low
 Iterations: 5
 Regularization Weight: 0.800000
 Processing Sampling: 4
 Output Sampling: 4
 Filter: Median
 Detrend: No
 Sectioning: 100.000000
 Baseline: Yes
 Scale to Raw Image: No
 Experimental PSF: No

3D Image Processing

3D Volume Projection = Precise
 Appearance = Threshold 9% (555), Threshold 3% (405), Ramp 91% (555), Ramp 97% (405), Maximum 100% both channels
 Background = Black
 Light = Brightness 152%, Azimuth 25°, Elongation 131°, Enabled Directional Lighting, Enabled Tone Mapping
 Projection = View Angle 35°, Scale Z 51%, Reverse Z-Axis NOT Selected, Stereo Anaglyph NOT Selected, Camera Separation 5% (deselected), Parallax Shift 0% (deselected)

Image Corrections

None


Image by P. Raut

Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE

Catalog	SA-000035
Stage	SIM²
Instrument	ZEISS Elyra 7
Microscope configuration	Zeiss Elyra 7, Andor1, AxioObserver, using Plan-Apochromat 63X/1.46 oil Korr M27 was used with the following parameters for each dye:
Structured source metadata values	62
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	66D65E32CC51CEFD739C97030831668E3C350EBB4F5DCE5109370ADE6A7FB7A6
Method PDF SHA-256	3C9C2901D3C41F836FDAEC7EC9CC04DE9D28377730078B7973A3C325CEE551B0

ORIGINAL IMAGE EVIDENCE / SINGLE-MOLECULE STORM

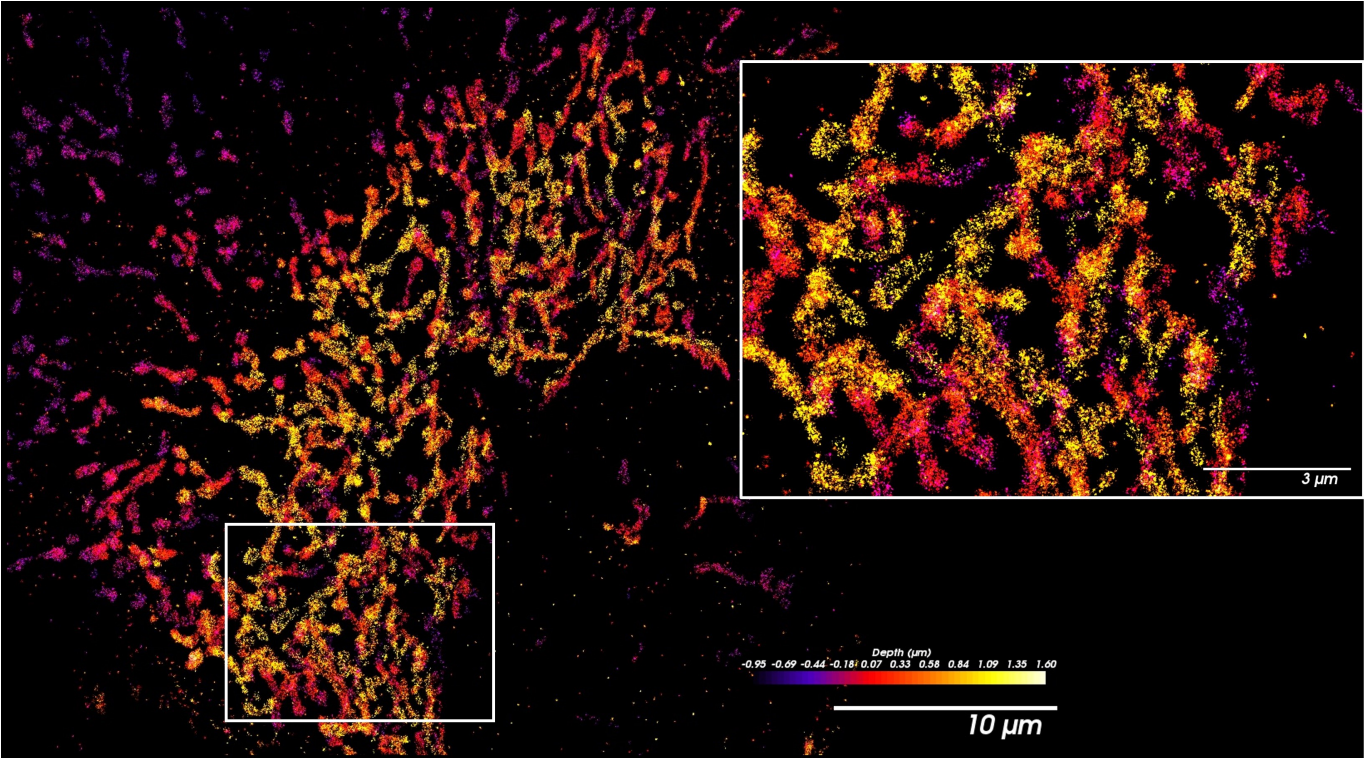

EVIDENCE TIER	Single-molecule STORM
INSTRUMENT	Bruker Vutara VXL
CELL MODEL	HeLa
DETECTED DYES	555
METADATA VALUES	79

STRUCTURED ACQUISITION METADATA / SINGLE-MOLECULE STORM

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Bruker Vutara VXL Biplane Single Molecule Microscope, using an Olympus 60X/1.30 silicon oil objective, was used with the following parameters:
Objective	Olympus 60X/1.30 silicon oil objective
Number of Probes	1
Number of Simultaneous Probes	1
Number of Reference Probes	1
Camera	Both Cameras
Color Channel	Both Channels
Probe Capture Mode	Interleaved
Z -Stack Capture Mode	Interleaved
Multiple Location Capture	Not selected
Post Record Reference	Not Selected
Fluidics	Not Selected
Autofocus Drift Correction	On
Biplane Module	635nm Dichroic
Objective	Silicon Selected
Stage Insert	Rectangular Selected
Course Focus Position	8-Well Chamber Selected
Dichroic	SuperRes
PSF	(Red, Orange)
Heater	Current: 26
Recording Vertical Field of View	100%
Widefield Camera Exposure Time	100ms 20ms
Super Resolution Camera Exposure Time	20ms
Widefield Camera Binning	1
Per-Probe Exposure Time	Selected
Predefined Probe	First probe: 555 nm (635 nm Dichroic); First reference probe: 555 nm (635 nm Dichroic)
Photoactivation/Imaging Laser	0% Selected
Exposure Time	20ms Selected
Record Workflow	Selected Options
View Mode	Widefield 200 µm
Capture Mode	Live
Piezo Current	178.5 µm

FIELD	SOURCE-DOCUMENTED VALUE
Widefield 555nm	0.1X Neutral Density Filter: Selected, @0.2% Laser Input
Reference Probe 1 Laser control (555 nm (635 nm Dichroic))	Not Selected
Widefield camera Exposure Time	100ms
Widefield Laser	"Widefield 555nm" was deselected, and "calibrate" under Autofocus was selected.
Current Intensity	4.5
Calibration Value	-5070 nm/unit
Autofocus Mode	Pre-Capture
SuperRes	50 µm is Selected
Piezo Record	Begin: 178.5; End: 178.5
SuperRes 555nm	0.1X Neutral Density Filter: Selected, @0.02% Laser Input
Record Workflow - Record Tab	Capture Parameters
Frames	Probe 1: 40000
Z Positions	1 using Steps: 0.1 µm (100nm)
Cycles	1
Time Points	1
Pause Between Cycles	Not Selected
Automatic Photoactivation Laser Control	Not Selected
Laser Power	90%
Cutout Width	16px
Max Frame Accumulation	1 frame
Max Accumulation Offset	1px
Fiducial at Max Accumulation	Not selected
Max Particles Per Frame	No Max
Background SLPE Removal	Not Selected
Cutout/Background Removal	Not Selected
Preview Cutout Positions	Selected
Probe1	BG threshold: 20
Sizing Mode	Constant
Particle size	20nm
Color by	Depth
Color Table	Single
Opacity Mode	Constant; Opacity 1: 0.3
Front-to-back Attenuation	Not Selected
Method	Particle (direct)
Time Intervals	10 Intervals

FIELD	SOURCE-DOCUMENTED VALUE
Pixel Size	50nm
Smoothing	8.00
PSF Z offset	-450 to +450
Radial precision	30
Axial precision	60
Clustering Algorithm	DBSCAN
Maximum Particle Distance	0.09µm (900nm)
Maximum Particle Count to Form Cluster	15
Computer Hulls	Not Selected
Compute Density Isosurfaces	Not Selected
Edit Settings	All Probes
Compute	Selected
Following Cluster Analysis Computation, under the Results Tab, ID Unassigned	Deselected

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit, IgG (H + L)

Cat ID# - SA 000035

Hela cells were grown on μ -Slide 8 Well high Glass Bottom Ibidi chamber, followed by -20°C methanol fixation and blocked with Thermo Fisher Fish Serum Blocker cat#37527X3. The primary antibody, Mitochondria Rabbit Recombinant Antibody (MTC02,2860R), was incubated for 1 hour at room temperature at a dilution of 1:100. Cells were washed 3X in PBS, and Identifyn® 555 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:200. Cells were washed 5X in PBS followed by the addition of Identifyn's™ proprietary STORM Buffer to the sample chamber enabling image acquisition.

Microscope

Bruker Vutara VXL Biplane Single Molecule Microscope, using an Olympus 60X/1.30 silicon oil objective, was used with the following parameters:

Calibration -

Calibration follows Identifyn's Calibration Standard Operating Procedure, which can be found here.

<https://identifyn.com/storm-calibration>

Image Acquisition -

SRX Software - Under the 'Single Molecule Localization' tab, 'Record' is selected and contains the following workflow tabs and parameters.

Configuration Tab - Capture Configuration

Number of Probes: 1

Number of Simultaneous Probes: 1

Number of Reference Probes: 1

Camera: Both Cameras

Color Channel: Both Channels

Probe Capture Mode: Interleaved

Z -Stack Capture Mode: Interleaved

Multiple Location Capture: Not selected

Post Record Reference: Not Selected

Fluidics: Not Selected

Autofocus Drift Correction: On

Microscope configuration

Biplane Module: 635nm Dichroic
 Objective: Silicon Selected
 Stage Insert: Rectangular Selected
 Course Focus Position: 8-Well Chamber Selected
 Dichroic: SuperRes
 PSF: (Red, Orange)
 Heater: Current: 26

Camera Configuration

Recording Vertical Field of View: 100%
 Widefield Camera Exposure Time: 100ms
 Super Resolution Camera Exposure Time: 20ms
 Widefield Camera Binning: 1
 Per-Probe Exposure Time: Selected

Probe Configuration

Predefined Probe: First probe: 555 nm (635 nm Dichroic); First reference probe: 555 nm (635 nm Dichroic)
 Photoactivation/Imaging Laser: 0% Selected
 Exposure Time: 20ms Selected

Experiment Configuration

Record Workflow: Selected Options
 View Mode: Widefield 200 μ m
 Capture Mode: Live

Stage and Piezo Selection

Examination of Sample

Cell(s) or Cellular Structure Localization - The red-bordered box identifies the area of the SuperRes view and defines a suitable cell(s) or cellular structure. The cell(s) or structures are optimally focused.

Piezo Current: 178.5 μ m

Probe 1 Laser control (555 nm (635 nm Dichroic))

Widefield 555nm: 0.1X Neutral Density Filter: Selected, @0.2% Laser Input
 Reference Probe 1 Laser control (555 nm (635 nm Dichroic): Not Selected

Advanced Tools Option

Widefield camera Exposure Time: 100ms
 Default values are maintained unless otherwise noted.

Widefield Laser: "Widefield 555nm" was deselected, and "calibrate" under Autofocus was selected.

Autofocus - Calibration Values

Current Position" -0.979

Current Intensity: 4.5

Calibration Value: -5070 nm/unit

Autofocus Mode: Pre-Capture

View Mode

SuperRes: 50 µm is Selected

Capture Mode

Live

Stage and Piezo Selection

Cell(s) or Cellular Structure Localization - Positioning of the target Cell or Subsection of the Target Cell is optimized and optimally focused.

Piezo Record: Begin: 178.5; End: 178.5

Probe 1 Laser control (555 nm (635 nm Dichroic)

SuperRes 555nm: 0.1X Neutral Density Filter: Selected, @0.02% Laser Input

Reference Probe 1 Laser control (555 nm (635 nm Dichroic)

Not Selected

Advanced Tools

Widefield Camera Exposure Time: 20ms

Default values are maintained unless otherwise noted.

Record Workflow - Record Tab: Capture Parameters

Frames: Probe 1: 40000

Z Positions: 1 using Steps: 0.1 µm (100nm)

Cycles: 1

Time Points: 1

Pause Between Cycles: Not Selected

Automatic Photoactivation Laser Control: Not Selected

Probe 1 Laser control (555 nm (635 nm Dichroic)

Laser Power: 90%

Expert Configuration Options - The Localization Tab

Beyond the values shown, all other parameters were default values.

Localization

Cutout Width: 16px
 Max Frame Accumulation: 1 frame
 Max Accumulation Offset: 1px
 Fiducial at Max Accumulation: Not selected
 Max Particles Per Frame: No Max
 Background SLPE Removal: Not Selected
 Cutout/Background Removal: Not Selected
 Preview Cutout Positions: Selected

Record Workflow - Localization Tab

Data Collection

The folder is created automatically with the localization file for this image acquisition.

Recording Summary

All parameters were carried over from previous tabs and are kept except:

Probe1: BG threshold: 20

Region of Interest

Not selected

Display

Was deployed to inspect if the BG threshold applied chooses localizations in an expected manner

Record Workflow - View Tab

Region of Interest

Default values

Visualization Parameters

Point Splatting
 Sizing Mode: Constant
 Particle size: 20nm
 Color by: Depth
 Color Table: Single
 Opacity Mode: Constant; Opacity 1: 0.3
 Front-to-back Attenuation: Not Selected

Post Acquisition analysis - View Tab

Drift Correction - Computed with the following parameters:

Method: Particle (direct)
 Time Intervals: 10 Intervals
 Pixel Size: 50nm
 Smoothing: 8.00

Advanced Particle Filters - Applied to the drift-corrected data with the following parameters

PSF Z offset: -450 to +450

Radial precision: 30

Axial precision: 60

The other parameters were not applied.

Statistical analysis - Computed to clean low background signals.

Statistics Dialog - Cluster Analysis

Clustering Algorithm: DBSCAN

Parameters

Maximum Particle Distance: 0.09µm (900nm)

Maximum Particle Count to Form Cluster: 15

Computer Hulls: Not Selected

Compute Density Isosurfaces: Not Selected

Edit Settings: All Probes

Compute: Selected


Following Cluster Analysis Computation, under the Results Tab, ID Unassigned: Deselected

Image by S. Thakur

Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE	
Catalog	SA-000035
Stage	Single-molecule STORM
Instrument	Bruker Vutara VXL
Microscope configuration	Bruker Vutara VXL Biplane Single Molecule Microscope, using an Olympus 60X/1.30 silicon oil objective, was used with the following parameters:
Structured source metadata values	79
Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	44147F5EFB724284081E0B31E39CCC89D44477E822B4C724163B7F8BA3168A5A
Method PDF SHA-256	F1588C5E6F19FAD35B833E6587610F6F28A8B41FCE5AEB3D6828A70DAD5E3EF0

ORIGINAL IMAGE EVIDENCE / CONTROL

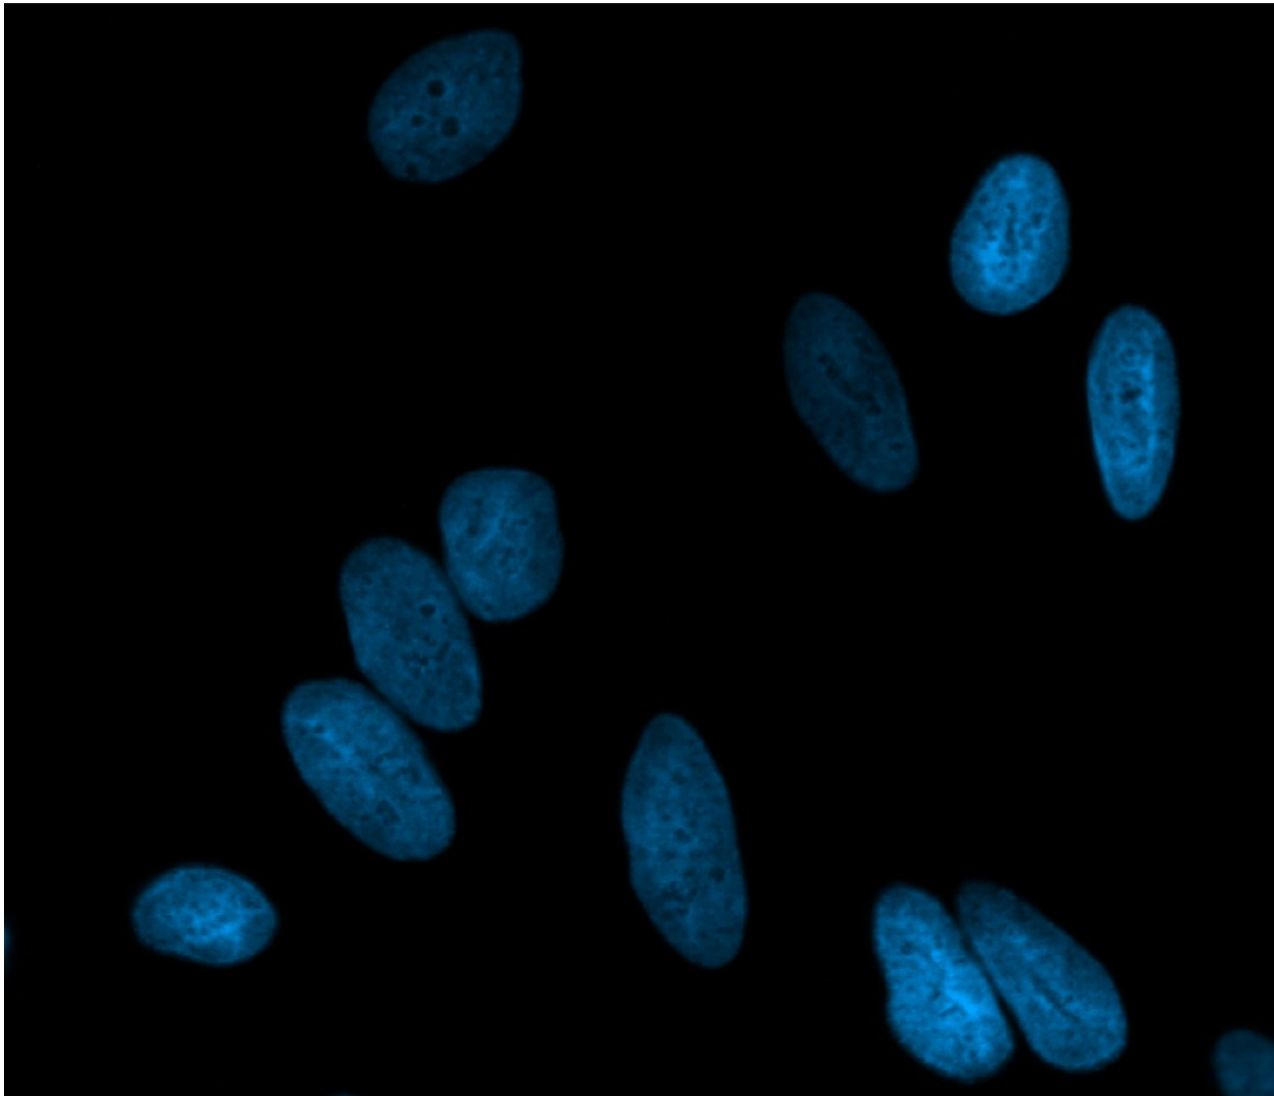

EVIDENCE TIER	Control
INSTRUMENT	ZEISS Axio Observer.Z1/7 Apotome
CELL MODEL	HeLa
DETECTED DYES	405/DAPI; 555
METADATA VALUES	32

STRUCTURED ACQUISITION METADATA / CONTROL

The values below were deterministically extracted from the preserved Identifyn method PDF text. They remain source-documented metadata, not new BENNETT measurements.

FIELD	SOURCE-DOCUMENTED VALUE
Platform / configuration	Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:
Objective	EC Plan-Neofluar 63X/1.25 oil M27
Channels	2
Scaling (Per Pixel)	0.143µm X 0.143µm
Image Size (Pixels)	1279 X 1100
Image Size (Scaled)	182.71µm X 157.14µm
Bit Depth	14 Bit
Image Center Position	X: 48.49mm, Y: 51.40mm
Stage Position	X: 48.49mm, Y: 51.40mm
ROI Center Offset	X: 1.14µm, Y: 0.00µm
Reflector	AF532-49014 49 DAPI
Beam Splitter	550 395
Filter Excitation Wavelength	515 - 545 335 - 383
Filter Emission Wavelength	555 - 595 420 - 470
Contrast Method	Fluorescence
Light source	X-Cite Xylis Lamp Intensity @25% X-Cite Xylis Lamp Intensity @10%
Exposure Time	200ms 30ms
Excitation Wavelength	553 353
Emission Wavelength	568 465
Effective NA	1.25
Imaging Device	Axiocam 807 mono
Camera Adapter	1X
Depth of Focus	1.10µm 0.90µm
Binning Mode	2,2
Apotome SIM Image Processing	Display Mode "Optical Sectioning" - enabled correction selected.

SOURCE METHOD

The text below is carried from the preserved Identifyn source record. Typography and pagination have been normalized for this preservation dossier; scientific wording has not been editorially rewritten.

Identifyn Standards for Optical Microscopy Methods™

Identifyn® SRM Alexa Fluor™ 555 Affinity Purified Goat Anti-Rabbit, IgG (H + L)

Cat ID# - SA 000035

Hela Cells were grown on acid-etched #1.5H cover glass to ~50% confluency, followed by -20°C methanol fixation and blocked with Thermo Fisher Fish Serum Blocker cat#37527X3. In the absence of a primary antibody, the Identifyn® 555 secondary antibody was incubated at room temperature for 1 hour at a dilution of 1:1000. Cells were washed 5X in PBS and mounted using ProLong™ Diamond Antifade Mountant with DAPI cat#P36962.

Microscope

Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:

Single Plane (2D)

Channels = 2

Scaling (Per Pixel) = 0.143µm X 0.143µm

Image Size (Pixels) = 1279 X 1100

Image Size (Scaled) = 182.71µm X 157.14µm

Bit Depth = 14 Bit

Image Center Position = X: 48.49mm, Y: 51.40mm

Stage Position = X: 48.49mm, Y: 51.40mm

ROI Center Offset = X: 1.14µm, Y: 0.00µm

555 -

Reflector = AF532-49014

Beam Splitter = 550

Filter Excitation Wavelength = 515 - 545

Filter Emission Wavelength = 555 - 595

Contrast Method = Fluorescence

Light source = X-Cite Xylis Lamp Intensity @25%

Exposure Time = 200ms

Excitation Wavelength = 553

Emission Wavelength = 568

Effective NA = 1.25

Imaging Device = Axiocam 807 mono

Camera Adapter = 1X

Depth of Focus = 1.10µm

Binning Mode = 2,2

DAPI -

Reflector = 49 DAPI
 Beam Splitter = 395
 Filter Excitation Wavelength = 335 - 383
 Filter Emission Wavelength = 420 - 470
 Contrast Method = Fluorescence
 Light source = X-Cite Xylis Lamp Intensity @10%
 Exposure Time = 30ms
 Excitation Wavelength = 353
 Emission Wavelength = 465
 Effective NA = 1.25
 Imaging Device = Axiocam 807 mono
 Camera Adapter = 1X
 Depth of Focus = 0.90µm
 Binning Mode = 2,2

Post Processing - SIM Processing

Apotome SIM Image Processing = Display Mode "Optical Sectioning" - enabled correction selected.

Normalization, Phase Corrector, Fourier Filter, and Deconvolution were NOT used.

Image Corrections

None

Control Summary -

In the absence of a primary antibody, Identifyn Standards for Optical Microscopy Methods™ were applied using standard staining methodology and image acquisition settings using the Zeiss Apotome SIM. With no image correction, the image demonstrates that the secondary antibody, minus a primary target, had no off-target binding and no significant presence of free dye within the sample.

The control data suggests the secondary antibody is highly specific and free of unconjugated (free) dye post-conjugation.

Image by J.K. Bennett

Copyright 2026 GMD12 LLC.

SOURCE PROVENANCE

Catalog	SA-000035
Stage	Control
Instrument	ZEISS Axio Observer.Z1/7 Apotome
Microscope configuration	Zeiss Axio Observer.Z1/7 Apotome SIM, using an EC Plan-Neofluar 63X/1.25 oil M27, Axiocam 807, and X-Cite Xylis Lamp was used with the following parameters for each dye:
Structured source metadata values	32

SOURCE PROVENANCE

Metadata source	PRESERVED_SOURCE_METHOD_PDF_TEXT
Cell model	HeLa
Image SHA-256	434D804C58F6AAAC1C49FCDBF8CC796A5C74918A5949CB9873D9BDACB094B416
Method PDF SHA-256	7A2052B91AC91BF366A75EA7C7301008F19C9E2722D93921810495992B9D816C